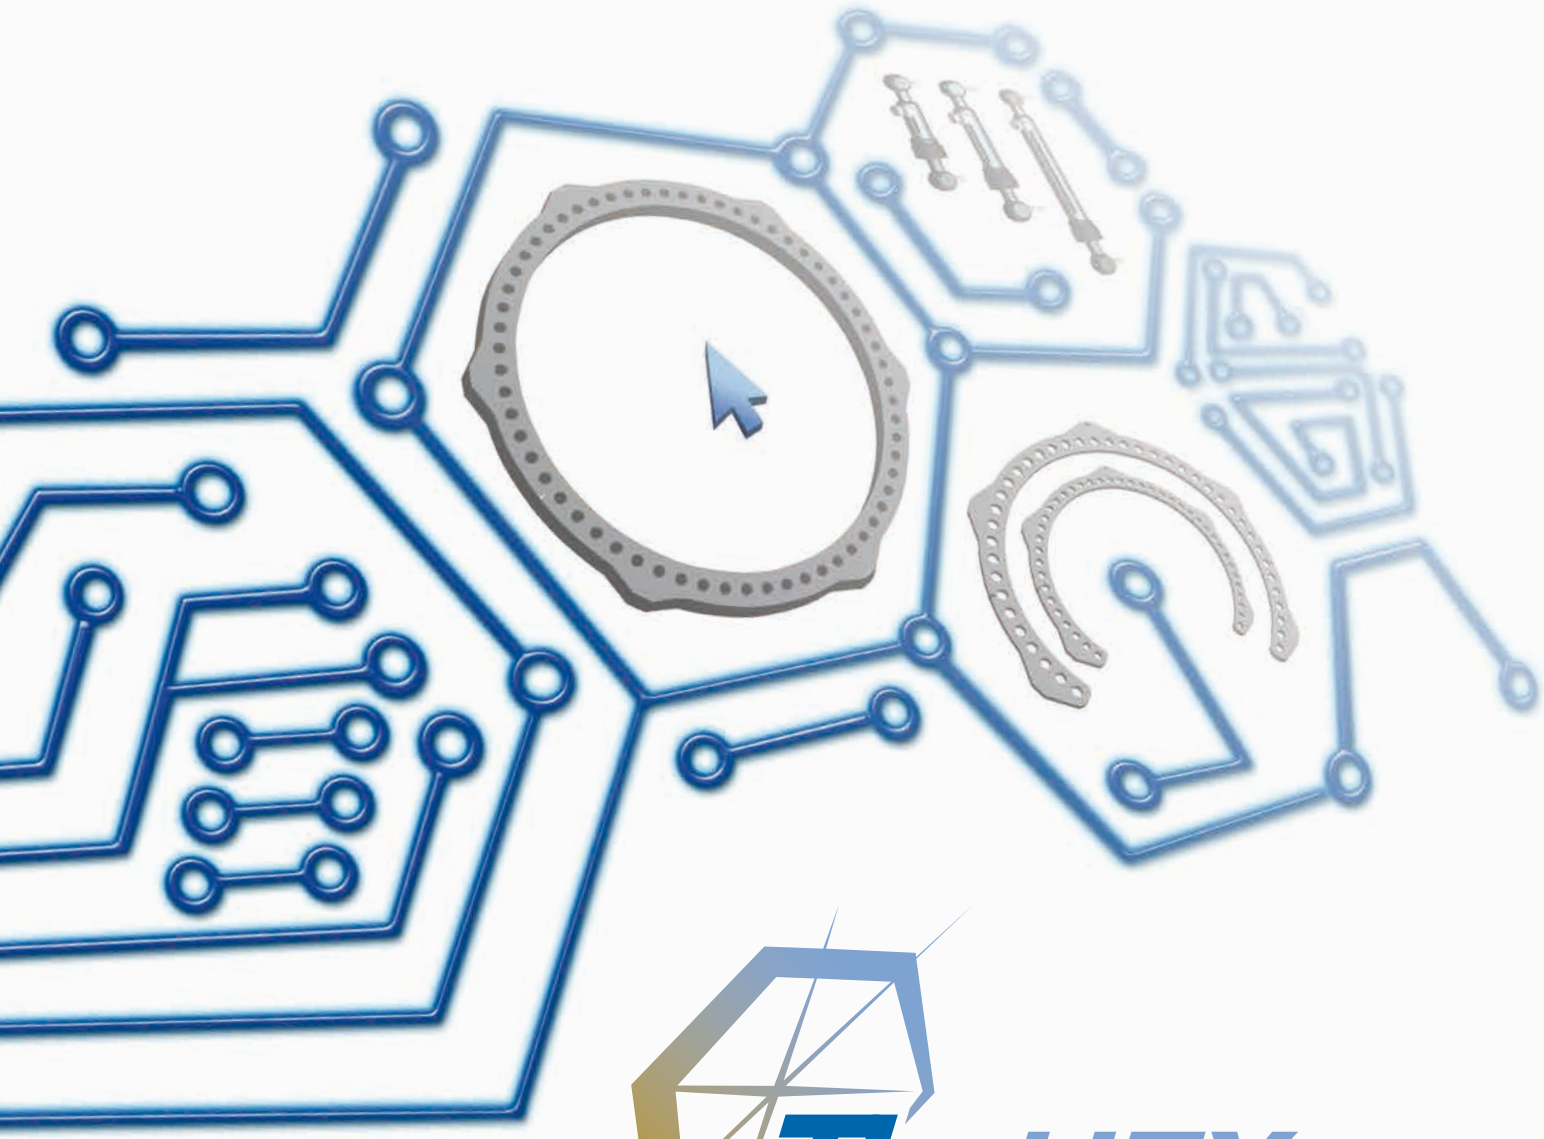

TL-HEX

TRUELOK HEXAPOD SYSTEM

Quick User's Guide

Software Version 1.3

ORTHOFIX®

WORKFLOW 1

1. REQUEST A NEW ACCOUNT 3

2. LOGIN PAGE 5

3. HOME PAGE 7

4. PATIENT → ADD A NEW PATIENT 7

4.1 ADD PRESCRIPTION PREFERENCES 7

5. PATIENT → LIST OF PATIENTS 9

5.1 SEARCH 9

6. CASE → LIST OF CASES 11

6.1 VIEW A CASE 11
6.2 SEND A CASE 13
6.3 ARCHIVE A CASE 13

7. CASE → ADD NEW CASE 15

8. DEFORMITY PARAMETERS 17

9. FRAME PARAMETERS 19

9.1 PREOPERATIVE MOUNTING PARAMETERS 21

10. POSTOPERATIVE 23

11. END OF CORRECTION 25

12. SCHEDULE 27

13. REPORT 29

13.1 PRESCRIPTION PDF 31
13.2 BOM PDF 31
13.3 REPORT PDF 33

14. CHECKUP 35

15. CHANGE PASSWORD 37

16. PRESCRIPTION PREFERENCES 37

WHAT IS NEW 38

Orthofix wishes to thank the following surgeons for their contribution to the development of this User's Guide:

Franz Birkholtz, M.D.

Alexander Cherkashin, M.D.

Mikhail Samchukov, M.D.

William Terrell, M.D.

The following provides a sequential overview of the process for a case management with TL-HEX software

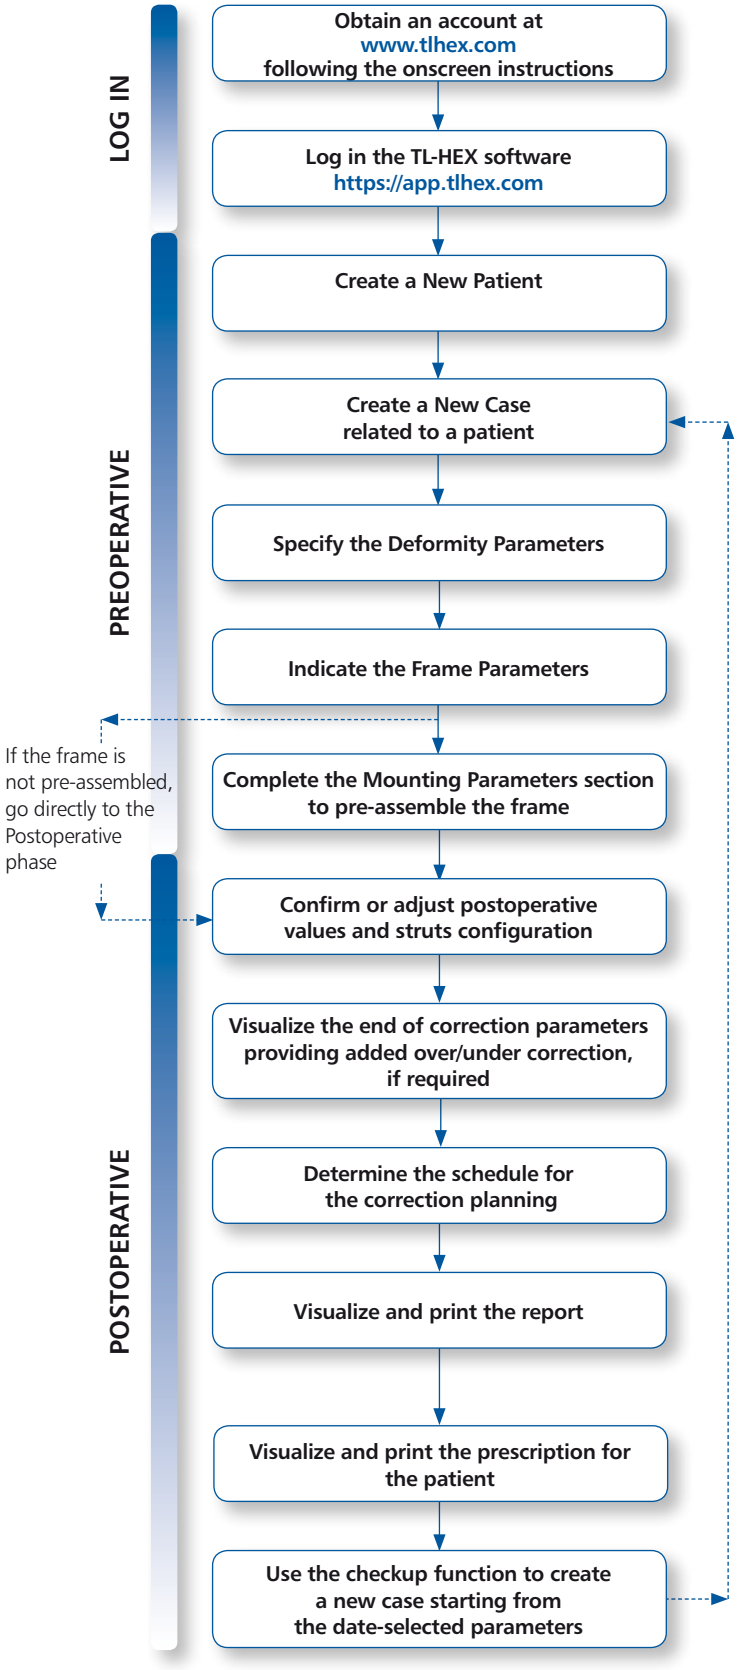

Access to the TL-HEX software is controlled by Username and Password. These can be obtained at www.tlhex.com by requesting a new account and following the onscreen instructions.
 # see screen 1 for details

Enter a valid Username and Password in the appropriate text fields and click Sign In to gain access to the software.
 # see screen 2 for details

In the Add New Patient screen, create a new patient if the patient doesn't exist. Each case must be linked to an existing patient.
 # see screen 4 for details

To start a new treatment, create a new case. Select patient from the ones available in the drop-down list providing the information required (Case Name, Case Number, Side, Bone Type).
 # see screen 7 for details

Describe the deformity starting from the reference segment identification. Then, provide the relevant parameters relative to the angular deformity, rotation, translation and bone length discrepancy.
 # see screen 8 for details

Indicate the ring type and size that will be used for the frame.
 # see screen 9 for details

If desired, complete this section with details of the planned frame position, relative to either the deformity apex or the osteotomy/fracture level. Strut types and lengths are being suggested.
 # see screen 9.1 for details

Provide the actual frame parameters and position as mounted and adjust/modify the struts configuration to adapt them to the configuration obtained during the surgery.
 # see screen 10 for details

Visualize the expected results at the end of correction.
If necessary, specify the eventual over/under correction parameters to be considered in the treatment.
 # see screen 11 for details

Define the schedule by specifying the latency period, the maximum rates and speeds of correction or the desired days of correction.
 # see screen 12 for details

Once all data is approved by the surgeon, the schedule will be calculated and the prescription is generated. The prescription can be saved and a hard copy will be given to the patient. For each correction step, the number of turns the patient must make are indicated for each strut for both acute and gradual adjustments. A hard copy of the bill of materials and the report may be generated. The report is a more detailed view for the surgeon indicating the length settings for the gradual and acute setting on the strut.
 # see screen 13 for details

Surgeon can use the checkup function to generate a new case starting from a specific date of the treatment. This new case will report all the parameters updated to the selected date. The Surgeon can then proceed to setup a new deformity correction treatment.
 # see screen 14 for details.

1

TL-HEX
TRUELOK HEXAPOD SYSTEM
ORTHOFIX
PRODUCT INFORMATION
TRAINING
FAQ
CONTACT US
The future of the hexapod system built on solid circular fixation experience
MEMBERS AREA
LOGIN
1
NEW USERS
Request an Account
2
PRIVACY POLICY | COOKIES | CONTACT US

1. Request a New Account	
	Description
1	Click [Login] to access the software if the account is already activated and the user has his/her own username and password
2	Click [Request an Account] button and follow the onscreen instructions to obtain a valid access to the TL-HEX software.

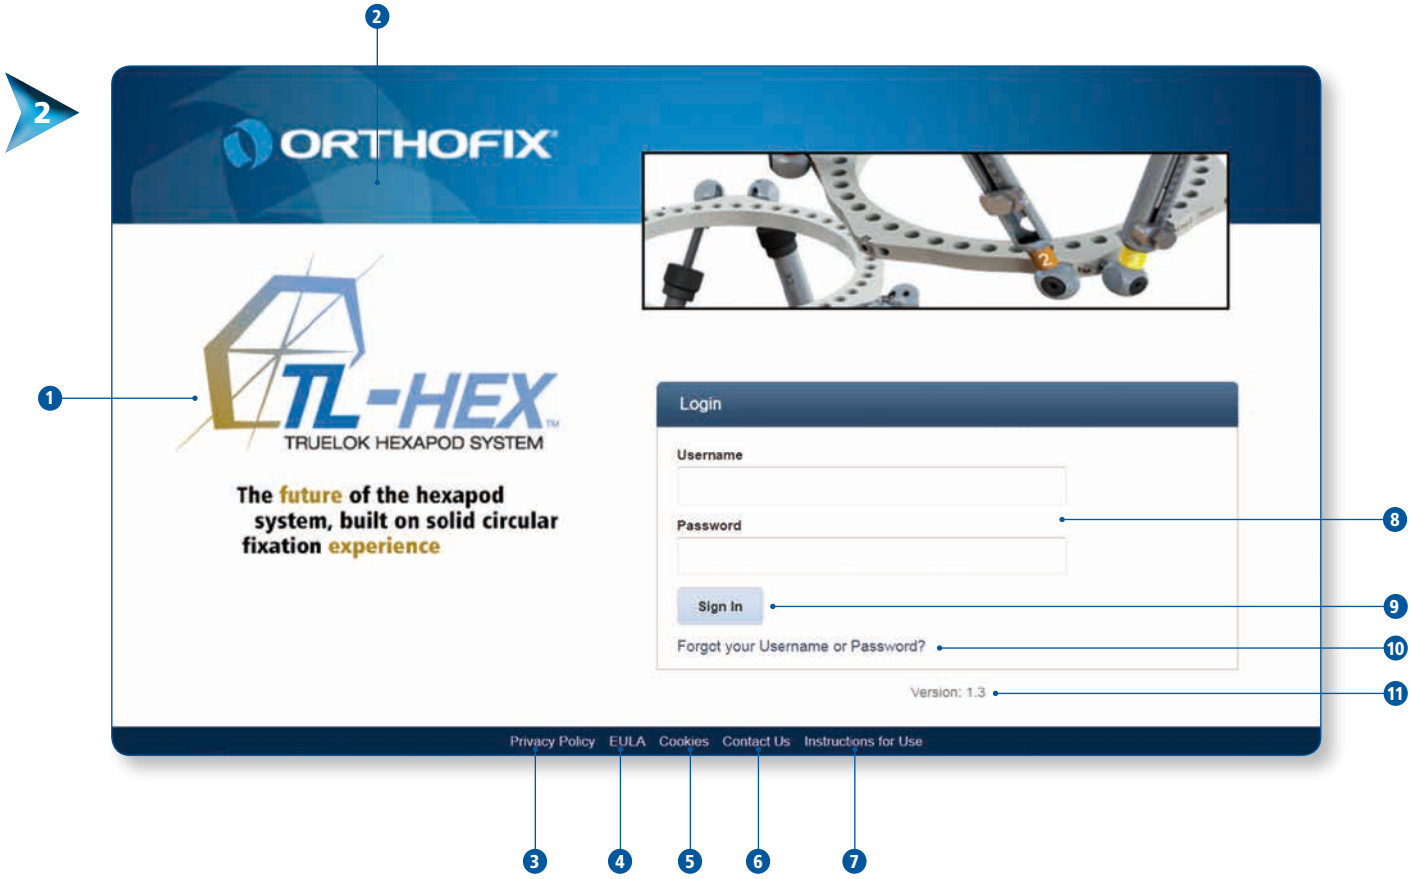
2
ORTHOFIX
TL-HEX
TRUELOK HEXAPOD SYSTEM
The future of the hexapod system, built on solid circular fixation experience
Login
Username
Password
Sign In
Forgot your Username or Password?
Version: 1.3
Privacy Policy
EULA
Cookies
Contact Us
Instructions for Use
1
2
3
4
5
6
7
8
9
10
11

2. Login Page	
	Description
This section is reported in all the application pages	
1	Click the TL-HEX logo to go to the product website www.tlhex.com
2	Click the Orthofix logo to go to the Company website intl.orthofix.com
FOOTER - This section is reported in all the application pages	
3	Click [Privacy Policy] to display the Privacy Policy statement
4	Click [EULA] to review the End User Licence Agreement subscribed for the application
5	Click [Cookies] to review the Cookies statement
6	Click [Contact us] to find how to contact the TL-HEX Customer Care support
7	Click [Instruction for Use] to access the TL-HEX support materials area
Login	
8	Enter a valid username and password in the appropriate text fields *Please note that username and password are case sensitive.*
9	Click [Sign In] button to access to the TL-HEX software
10	Click the link *Forgot your Username or Password?* and follow the displayed instructions to recover username and/or password
11	Check the version of the SW

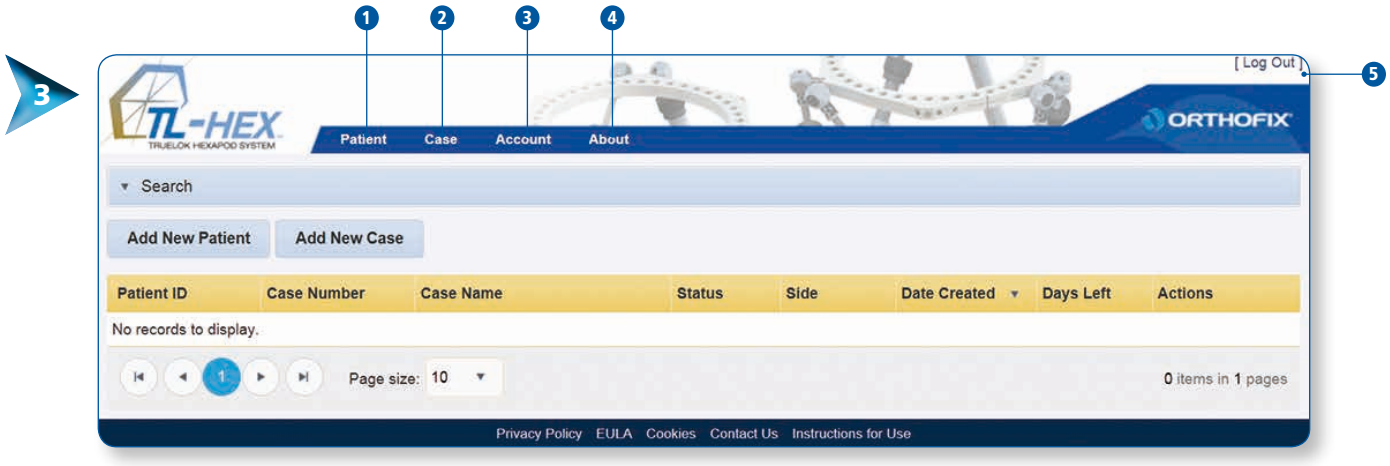
3
1
2
3
4
5
TL-HEX
TRUELOK HEXAPOD SYSTEM
Patient
Case
Account
About
[Log Out]
ORTHOFIX
Search
Add New Patient
Add New Case
Patient ID
Case Number
Case Name
Status
Side
Date Created
Days Left
Actions
No records to display.
Page size: 10
0 items in 1 pages
Privacy Policy
EULA
Cookies
Contact Us
Instructions for Use

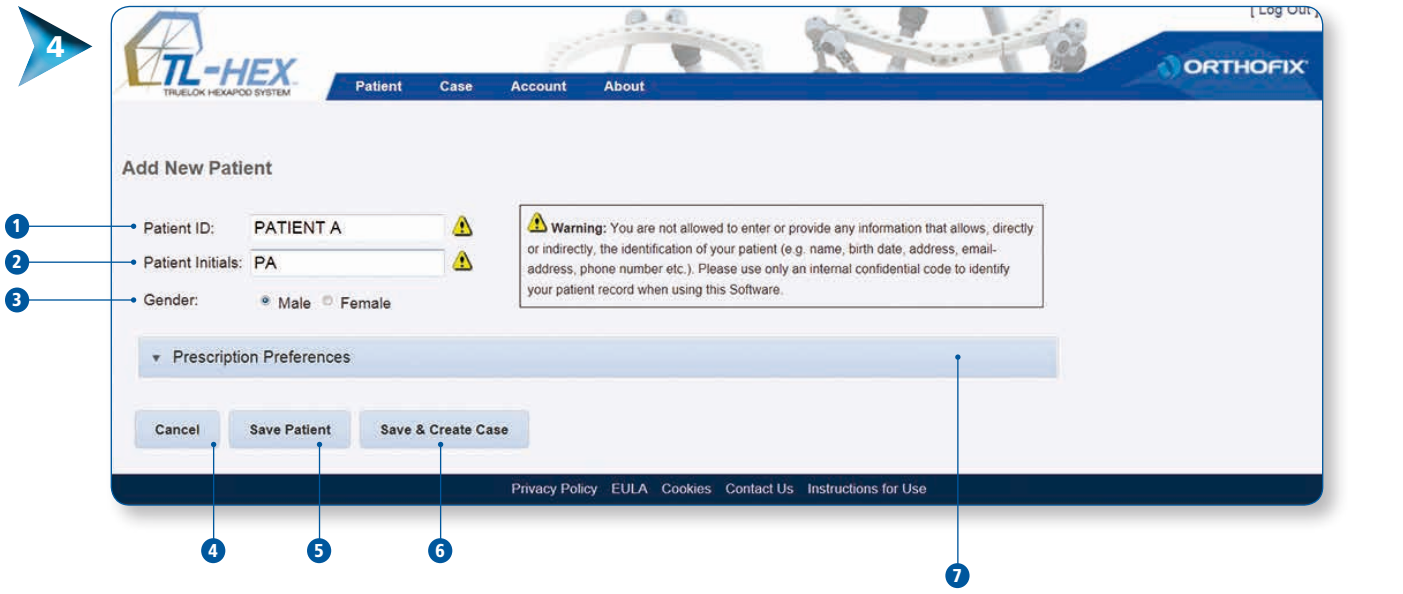
4
TL-HEX
TRUELOK HEXAPOD SYSTEM
Patient
Case
Account
About
ORTHOFIX
Add New Patient
1
Patient ID:
PATIENT A
2
Patient Initials:
PA
3
Gender:
Male
Female
Warning: You are not allowed to enter or provide any information that allows, directly or indirectly, the identification of your patient (e.g. name, birth date, address, email-address, phone number etc.). Please use only an internal confidential code to identify your patient record when using this Software.
Prescription Preferences
Cancel
Save Patient
Save & Create Case
Privacy Policy
EULA
Cookies
Contact Us
Instructions for Use
4
5
6
7

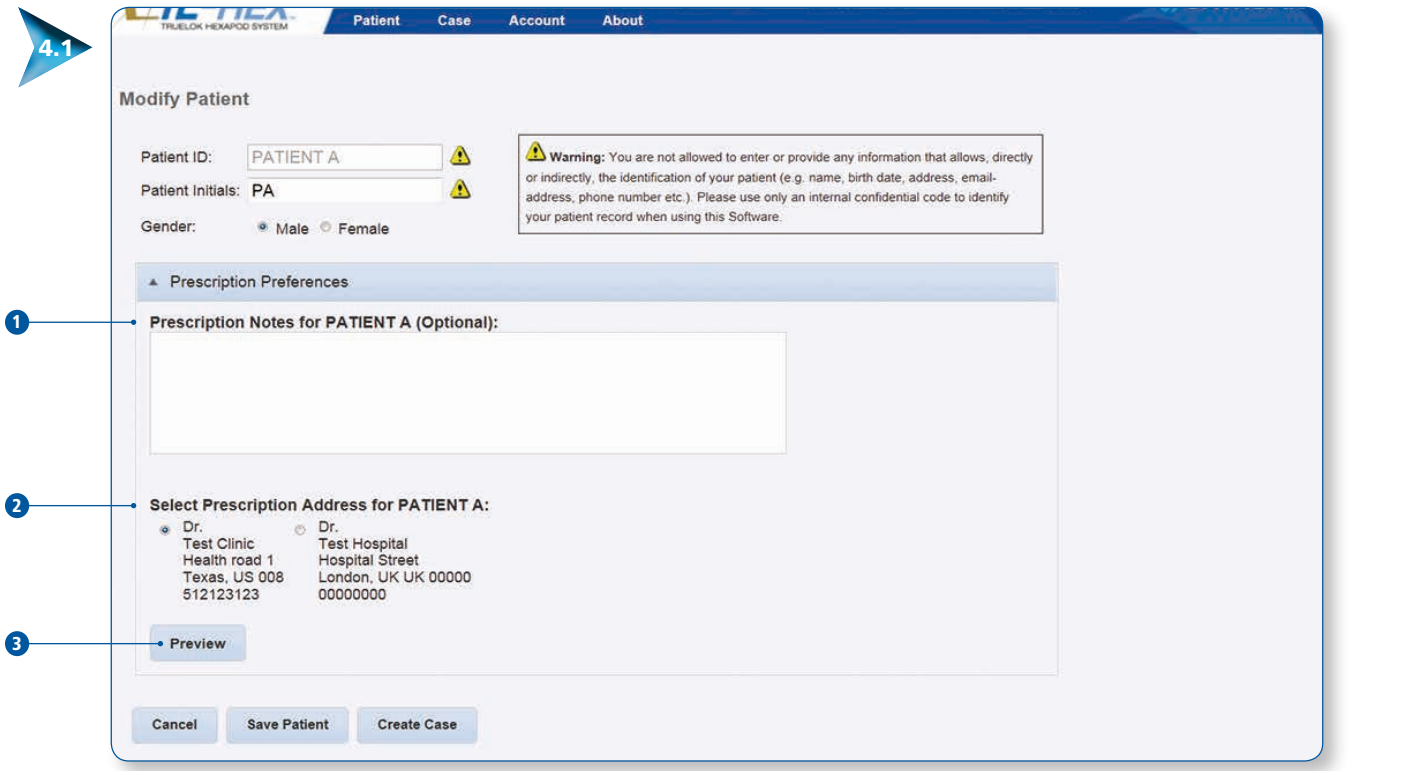
4.1
TL-HEX
TRUELOK HEXAPOD SYSTEM
Patient
Case
Account
About
Modify Patient
Patient ID:
PATIENT A
Patient Initials:
PA
Gender:
Male
Female
Warning: You are not allowed to enter or provide any information that allows, directly or indirectly, the identification of your patient (e.g. name, birth date, address, email-address, phone number etc.). Please use only an internal confidential code to identify your patient record when using this Software.
Prescription Preferences
1
Prescription Notes for PATIENT A (Optional):
2
Select Prescription Address for PATIENT A:
Dr.
Test Clinic
Health road 1
Texas, US 008
512123123
Dr.
Test Hospital
Hospital Street
London, UK UK 00000
00000000
3
Preview
Cancel
Save Patient
Create Case

3. Home Page	
MENU STRUCTURE - Reported in all the application pages when user is logged in	
	Description
1	Click [Patient] to access to the Patients Menu functionalities • Select [List of Patient] to view all the registered patients (see screen N°.5 for details) • Select [Add New Patient] to start a new patient registration (see screen N°.4 for details) All cases are related to a patient, therefore a new patient who doesn't exist must be created prior to begin a new case.
2	Click [Case] to access to the Cases Menu functionalities • Select [List of Cases] to view all the cases (see screen N°.6 for details) • Select [Add New Case] to start a new case (see screen N°.7 for details)
3	Click [Account] to access to the Account Menu functionalities * Select [Account Information] to view the registered information about the account * Select [Prescription Preferences] to view and manage other addresses related to this account (see screen N°. 16 for details) • Select [Change password] to invoke the change password procedure (see screen N°.15 for details)
4	Click [About] to view more information about the product
5	Click on [Log Out] to disconnect from the application

4. Patient → Add New Patient	
	Description
1	Insert the Patient ID
2	Insert Patient Initials or other reference associated with the patient
3	Select Patient Gender • Male - or - • Female
4	By clicking [Cancel] all the entered information is discarded and the application returns to the List of Patients screen (see screen N°.5 for details)
5	Click [Save Patient] to create a new patient and move to the List of Patients screen (see screen N°.5 for detail)
6	Click [Save & Create Case] to create a new patient and a brand new case linked to it. You will be promptly redirect to Add New Case screen (see screen N° 7 for details)
7	Expand [Prescription Preferences] to choose a set of contact information that will be displayed on the prescription pdf
⚠	**Warning:** Under the Orthofix Terms of Use, the surgeon should never enter information that directly identifies a patient. The patient number is intended to be used as an identifying link to the patient within the surgeon's patient management system.

4.1 Add Prescription Preferences	
	Description
1	Enter some (optional) notes related to this Patient ID
2	Choose the address to be displayed on the prescription pdf for this patient
3	Click on [Preview] to have a sample of the Prescription Preferences on the prescription pdf

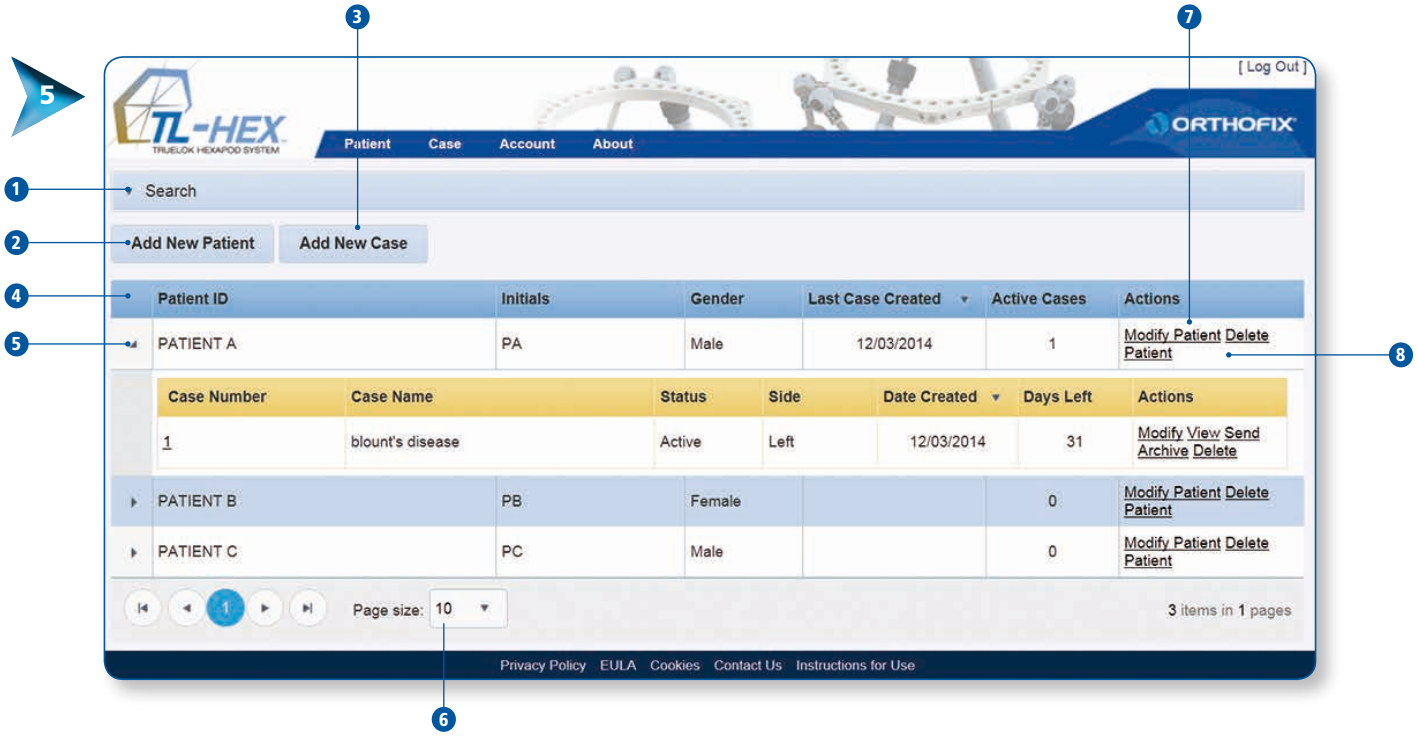
5
[Log Out]
TL-HEX
TRUELOK HEXAPOD SYSTEM
Patient
Case
Account
About
ORTHOFIX
1 Search
2 Add New Patient
Add New Case
3
4
5
6
7
8
Patient ID
Initials
Gender
Last Case Created
Active Cases
Actions
PATIENT A
PA
Male
12/03/2014
1
Modify Patient Delete Patient
Case Number
Case Name
Status
Side
Date Created
Days Left
Actions
1
blount's disease
Active
Left
12/03/2014
31
Modify View Send Archive Delete
PATIENT B
PB
Female
0
Modify Patient Delete Patient
PATIENT C
PC
Male
0
Modify Patient Delete Patient
Page size: 10
3 items in 1 pages
Privacy Policy EULA Cookies Contact Us Instructions for Use

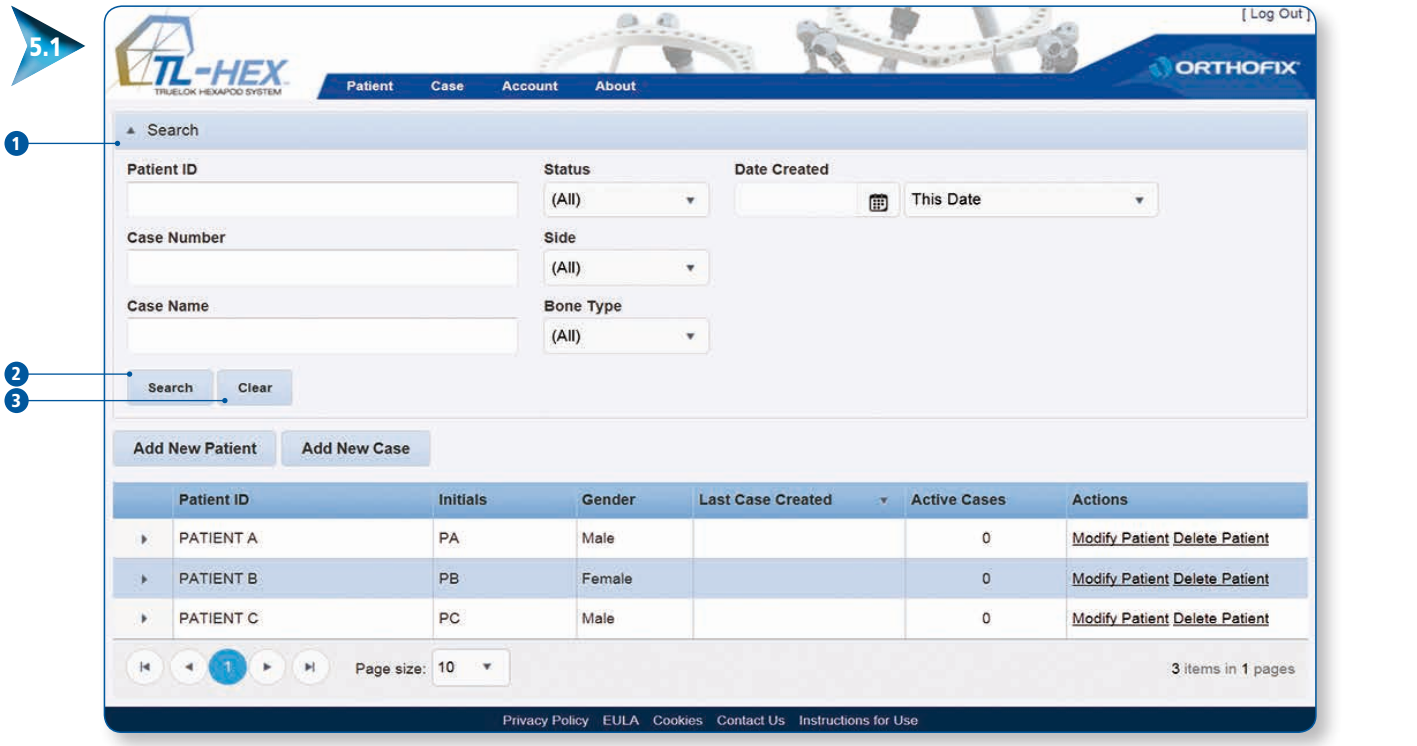
5.1
[Log Out]
TL-HEX
TRUELOK HEXAPOD SYSTEM
Patient
Case
Account
About
ORTHOFIX
1 Search
Patient ID
Status
(All)
Date Created
This Date
Case Number
Side
(All)
Case Name
Bone Type
(All)
2 Search
3 Clear
Add New Patient
Add New Case
Patient ID
Initials
Gender
Last Case Created
Active Cases
Actions
PATIENT A
PA
Male
0
Modify Patient Delete Patient
PATIENT B
PB
Female
0
Modify Patient Delete Patient
PATIENT C
PC
Male
0
Modify Patient Delete Patient
Page size: 10
3 items in 1 pages
Privacy Policy EULA Cookies Contact Us Instructions for Use

5. Patient ➔ List of Patients	
	Description
1	Expand [Search] bar in order to search through the list of patients using a set of specific criteria
2	Click [Add New Patient] to create a new patient (see screen N°.4 for details)
3	Click [Add New Case] to start a new case (see screen N°.7 for details)
4	Click on any of the header (a part from "Action") to sort the list accordingly
5	Click on the arrow near a Patient ID to expand the list of cases related to it
6	Navigate through the list of patients using the arrow and set the number of patients you want to display on a page using the page size drop down
7	Click "Modify Patient" to edit patient details
8	Click "Delete Patient" to delete definitively a Patient. The application prompts for a confirmation of the deletion. **Delete cannot be undone and implies that all the cases related to that patient will be deleted.**

5.1 List of Patients -> Search	
	Description
1	Enter one or more search criteria.
2	Click on [Search] to view the results
3	Click on [Clear] to cancel all the search criteria

6

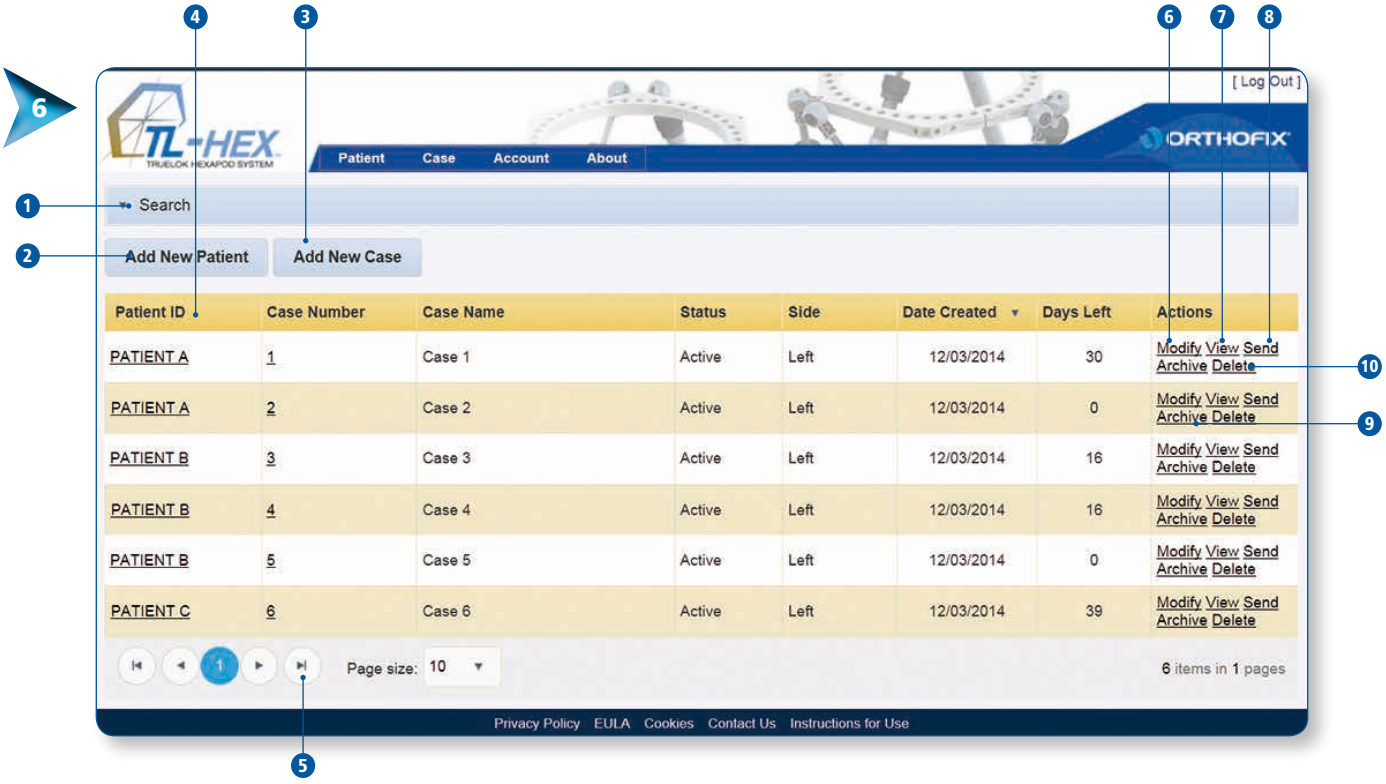
[Log Out]
TL-HEX
TRUELOK HEXAPOD SYSTEM
ORTHOFIX
Patient
Case
Account
About
Search
Add New Patient
Add New Case
Patient ID
Case Number
Case Name
Status
Side
Date Created
Days Left
Actions
PATIENT A 1 Case 1 Active Left 12/03/2014 30 Modify View Send Archive Delete
PATIENT A 2 Case 2 Active Left 12/03/2014 0 Modify View Send Archive Delete
PATIENT B 3 Case 3 Active Left 12/03/2014 16 Modify View Send Archive Delete
PATIENT B 4 Case 4 Active Left 12/03/2014 16 Modify View Send Archive Delete
PATIENT B 5 Case 5 Active Left 12/03/2014 0 Modify View Send Archive Delete
PATIENT C 6 Case 6 Active Left 12/03/2014 39 Modify View Send Archive Delete
Page size: 10
6 items in 1 pages
Privacy Policy EULA Cookies Contact Us Instructions for Use
1
2
3
4
5
6
7
8
9
10

6.1

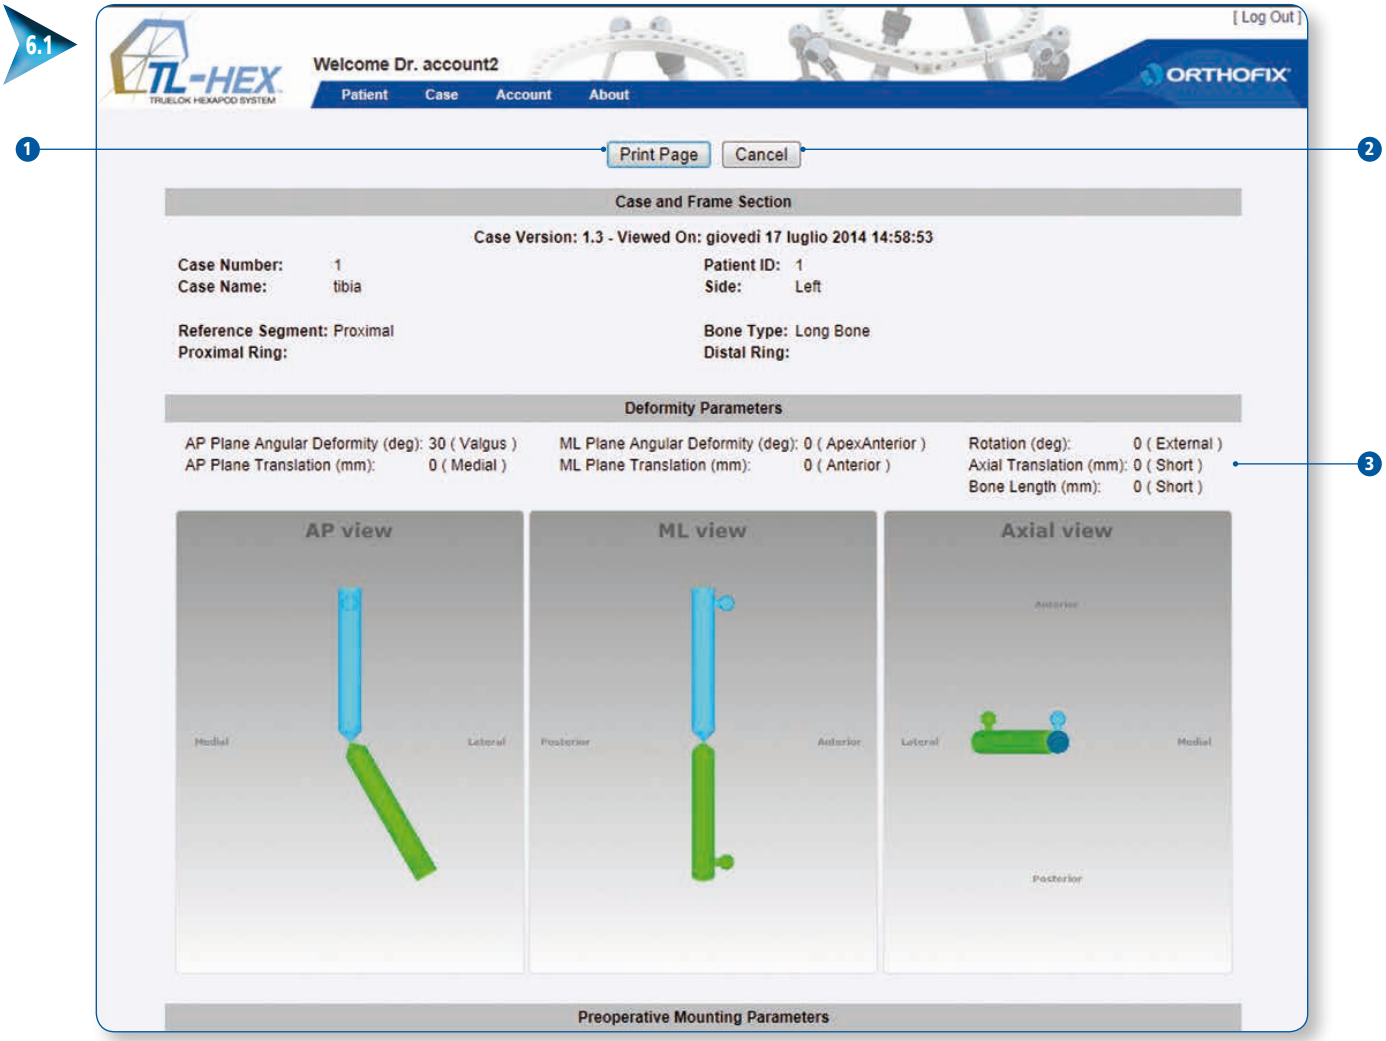
[Log Out]
TL-HEX
TRUELOK HEXAPOD SYSTEM
Welcome Dr. account2
ORTHOFIX
Patient
Case
Account
About
Print Page
Cancel
Case and Frame Section
Case Version: 1.3 - Viewed On: giovedì 17 luglio 2014 14:58:53
Case Number: 1
Case Name: tibia
Patient ID: 1
Side: Left
Reference Segment: Proximal
Proximal Ring:
Bone Type: Long Bone
Distal Ring:
Deformity Parameters
AP Plane Angular Deformity (deg): 30 (Valgus)
AP Plane Translation (mm): 0 (Medial)
ML Plane Angular Deformity (deg): 0 (ApexAnterior)
ML Plane Translation (mm): 0 (Anterior)
Rotation (deg): 0 (External)
Axial Translation (mm): 0 (Short)
Bone Length (mm): 0 (Short)
AP view
ML view
Axial view
Preoperative Mounting Parameters
1
2
3

6. Case →List of Cases	
	Description
1	Expand [Search] bar in order to search through the list of cases using a set of specific criteria (see screen N°. 5.1 for details)
2	Click [Add New Patient] to create a new patient (see screen N°.4 for details)
3	Click [Add New Case] to start a new case (see screen N°.7 for details)
4	Click on any of the header (a part from "Action") to sort the list accordingly
5	Navigate through the list of cases using the arrow and set the number of cases you want to display on a page using the page size drop down
6	Click on [Modify] to make changes to a case. You cannot modify received or archived cases
7	Click on [View] to see a read-only version of a case (see screen N°. 6.1 for details)
8	Click on [Send] to send a case to another TI-HEX SW user (see screen N°. 6.2 for details). You cannot send a received case
9	Click on [Archive] to close a case and make it read-only (see screen N°. 6.3 for details). This action cannot be undone. You cannot archive a sent case
10	Click on [Delete] to delete a case. Delete action cannot be undone

6.1 View a Case	
	Description
1	Click [Print Page] to print a summary of the full case
2	Click [Cancel] to go back to the list of cases
3	The summary displays all the details about the deformity, the frame and the prescription along with the AP, ML and Axial views

6.2

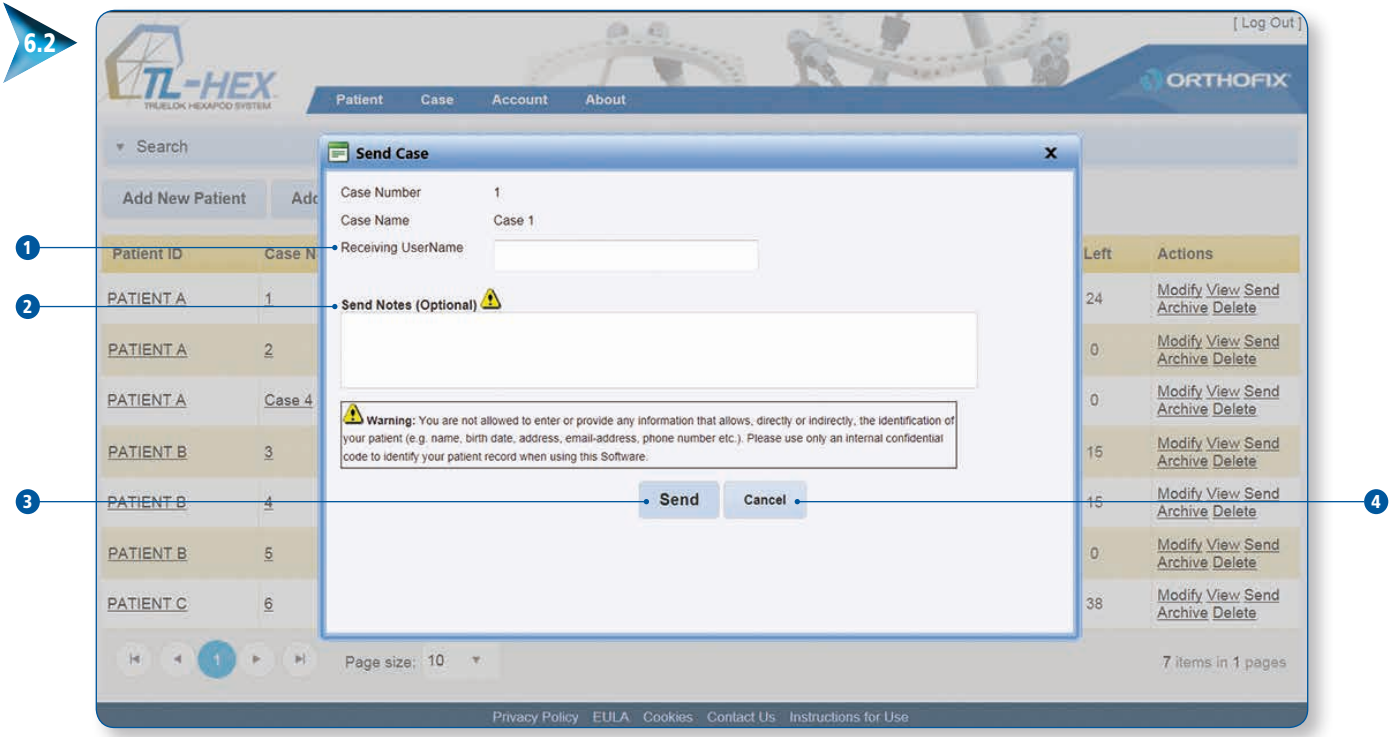
[Log Out]
TL-HEX
TRUELOK HEXAPOD SYSTEM
ORTHOFIX
Patient
Case
Account
About
Search
Add New Patient
Send Case
Case Number 1
Case Name Case 1
Receiving UserName
Send Notes (Optional)
Warning: You are not allowed to enter or provide any information that allows, directly or indirectly, the identification of your patient (e.g. name, birth date, address, email-address, phone number etc.). Please use only an internal confidential code to identify your patient record when using this Software.
Send
Cancel
Patient ID
Case N
Left
Actions
PATIENT A 1 24 Modify View Send Archive Delete
PATIENT A 2 0 Modify View Send Archive Delete
PATIENT A Case 4 0 Modify View Send Archive Delete
PATIENT B 3 15 Modify View Send Archive Delete
PATIENT B 4 15 Modify View Send Archive Delete
PATIENT B 5 0 Modify View Send Archive Delete
PATIENT C 6 38 Modify View Send Archive Delete
Page size: 10
7 items in 1 pages
Privacy Policy EULA Cookies Contact Us Instructions for Use
1
2
3
4

6.3

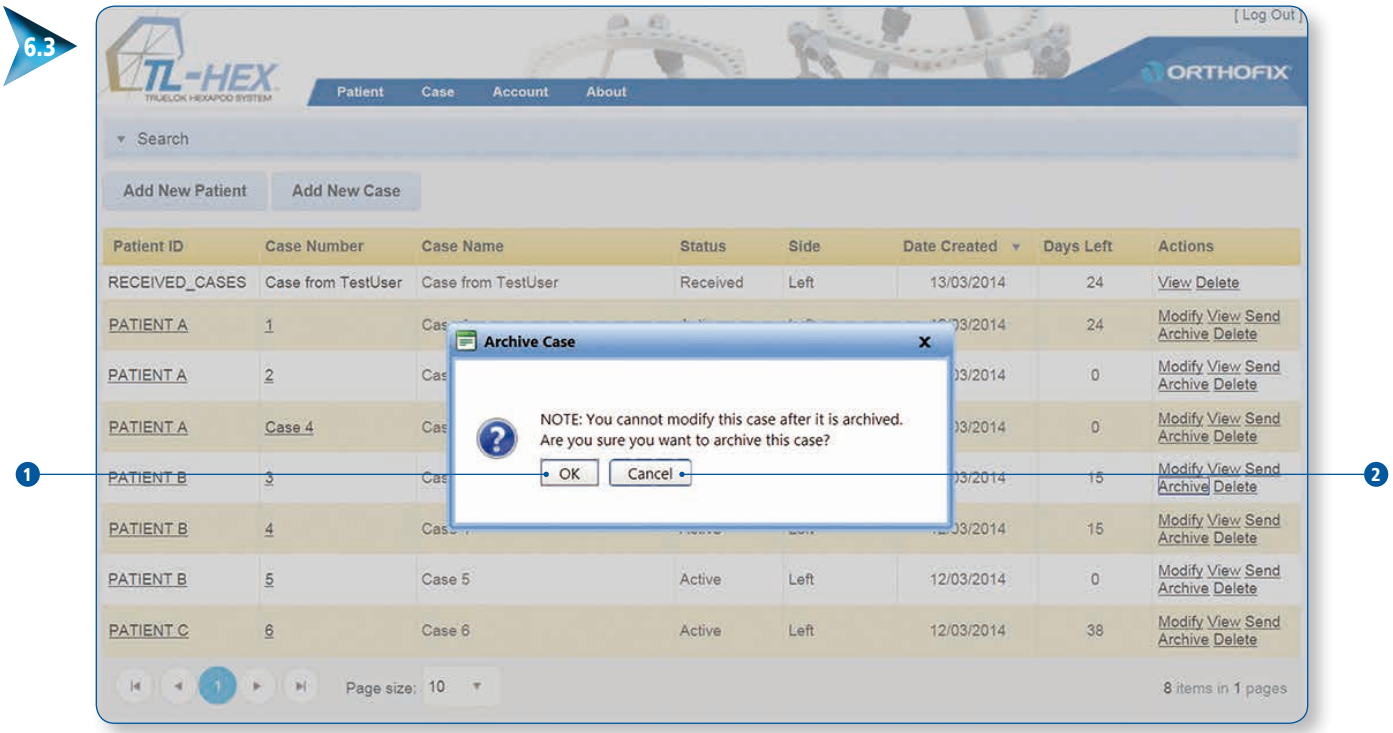
[Log Out]
TL-HEX
TRUELOK HEXAPOD SYSTEM
ORTHOFIX
Patient
Case
Account
About
Search
Add New Patient
Add New Case
Patient ID
Case Number
Case Name
Status
Side
Date Created
Days Left
Actions
RECEIVED_CASES Case from TestUser Case from TestUser Received Left 13/03/2014 24 View Delete
PATIENT A 1 24 Modify View Send Archive Delete
PATIENT A 2 0 Modify View Send Archive Delete
PATIENT A Case 4 0 Modify View Send Archive Delete
PATIENT B 3 15 Modify View Send Archive Delete
PATIENT B 4 15 Modify View Send Archive Delete
PATIENT B 5 Case 5 Active Left 12/03/2014 0 Modify View Send Archive Delete
PATIENT C 6 Case 6 Active Left 12/03/2014 38 Modify View Send Archive Delete
Archive Case
NOTE: You cannot modify this case after it is archived.
Are you sure you want to archive this case?
OK
Cancel
Page size: 10
8 items in 1 pages
1
2

6.2 Send a Case	
	Description
1	Enter the Username of the receiver
2	Optionally enter some notes
3	Click [Send] to send the case
4	Click [Cancel] to annul the action and go back to list of cases

6.3 Archive a Case	
	Description
1	Click [OK] to archive a case and make it read-only.**You cannot revert this action**
2	Click [Cancel] to annul this action

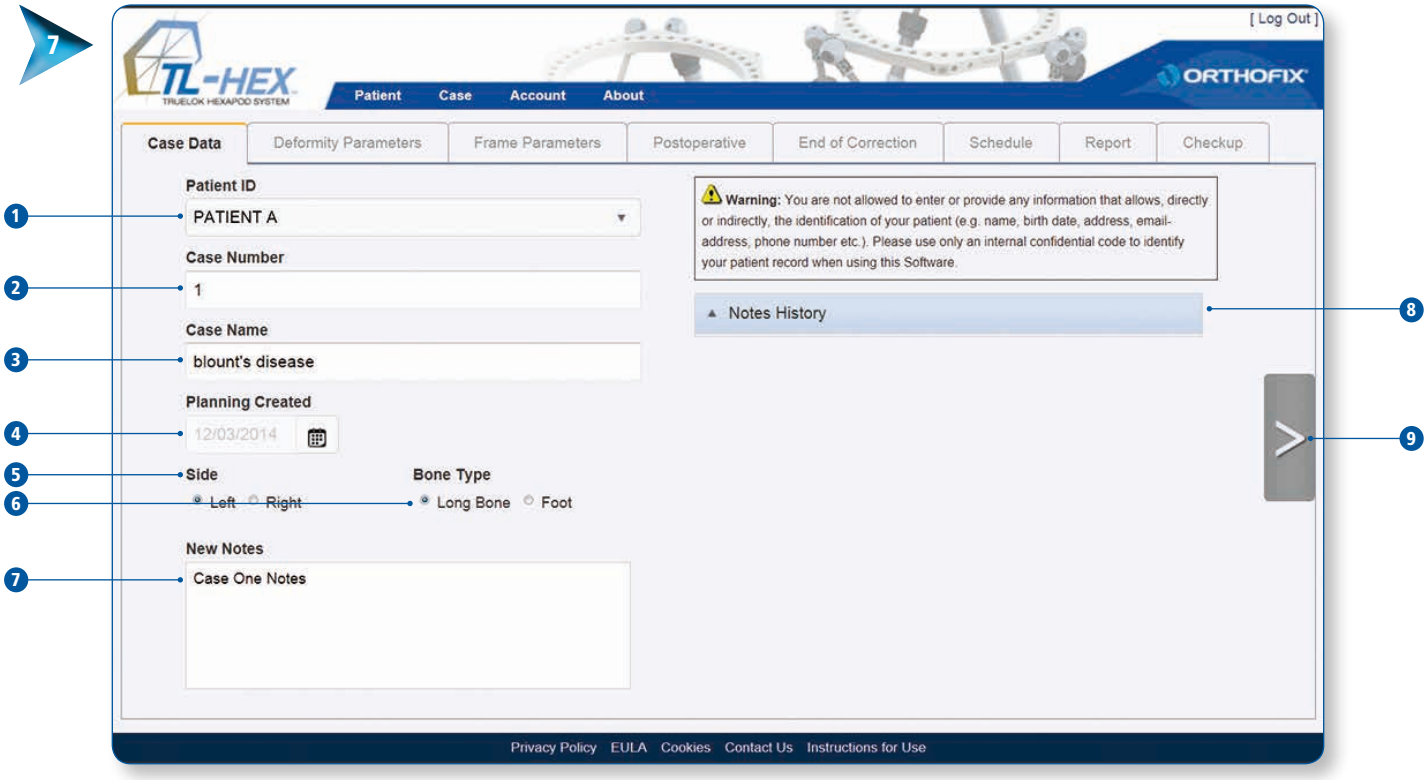
7
[Log Out]
TL-HEX
TRUELOK HEXAPOD SYSTEM
Patient
Case
Account
About
ORTHOFIX
Case Data
Deformity Parameters
Frame Parameters
Postoperative
End of Correction
Schedule
Report
Checkup
Patient ID
PATIENT A
Case Number
1
Case Name
blount's disease
Planning Created
12/03/2014
Side
Left
Right
Bone Type
Long Bone
Foot
New Notes
Case One Notes
Warning: You are not allowed to enter or provide any information that allows, directly or indirectly, the identification of your patient (e.g. name, birth date, address, email-address, phone number etc.). Please use only an internal confidential code to identify your patient record when using this Software.
Notes History
Privacy Policy
EULA
Cookies
Contact Us
Instructions for Use
1
2
3
4
5
6
7
8
9

7. Case → Add New Case	
	Description
1	Select the Patient from the drop-down selector. If no patients have been entered, the drop-down selector will be empty. To create a Patient before beginning a case creation see screen N°.4 for details
2	Assign the Case Number
3	Specify the Case Name (reference associated with this case)
4	Select the Planning Date by clicking the calendar icon
5	Select the side • Left - or - • Right
6	Select the Bone Type • Long Bone - or - • Foot
7	Specify additional notes, if any
8	Review the inserted notes, if they exist
9	Click [Next] to proceed with the next steps in the treatment planning process [Deformity Parameters]
⚠	**Warning:** Under the Orthofix Terms of Use, the surgeon should never enter information that directly identifies a patient. The patient number is intended to be used as an identifying link to the patient within the surgeon's patient management system

8
4
7
[Log Out]
TL-HEX
TRUELOK HEXAPOD SYSTEM
ORTHOFIX
Patient
Case
Account
About
1
Case Number: 1
Case Name: Case 1
Patient ID: PATIENT A
Side: Left
Bone Type: Long Bone
Case Data
Deformity Parameters
Frame Parameters
Postoperative
End of Correction
Schedule
Report
Checkup
2
Reference Segment
Proximal
Distal
Rotation (deg)
0
External
Internal
5
3
AP Plane Angular Deformity (deg)
0
Valgus
Varus
ML Plane Angular Deformity (deg)
0
Apex Anterior
Apex Posterior
Axial Translation (mm)
0
Short
Long
8
6
AP Plane Translation (mm)
0
Medial
Lateral
ML Plane Translation (mm)
0
Anterior
Posterior
Optional Bone Length (mm)
0
Short
Long
Update Views
9
AP view
ML view
Axial view
11
12
10
Privacy Policy
EULA
Cookies
Contact Us
Instructions for Use

8. Deformity Paramaters	
	Description
1	Summary of Case Data provided in the Case Data tab
Deformity Parameters	
2	Choose the reference segment as • Proximal - or - • Distal Refer to the Fig. 1 for the description of the moving bone segment translation depending on proximal or distal location of the reference segment. 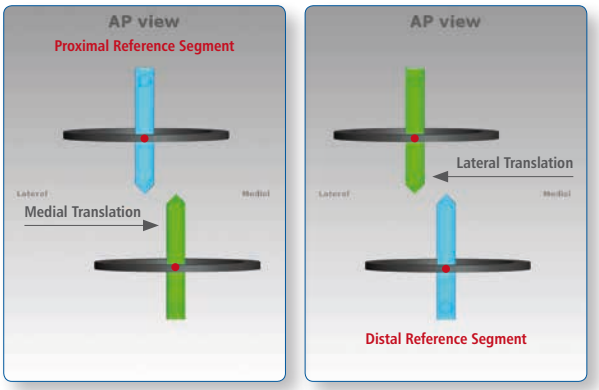 Fig. 1 In the software diagram [10], the reference segment is colored in blue while the moving segment is colored in green
ANGULATION	
3	Insert *coronal plane* angulation (AP view) in degrees. This can be either • Valgus - or • Varus, depending whether the distal segment is bent towards or away from the midline
4	Insert *sagittal plane* angulation (MP view) in degrees. It is described as • Apex Anterior (procurvatum) - or- • Apex Posterior (recurvatum)
5	Insert horizonal plane angulation (Axial view) in degrees. It is described as • External rotation - or - • Internal rotation
TRANSLATION	
6	Insert *coronal plane* translation (AP view) in mm. It is described as • Medial - or - • Lateral
7	Insert *sagittal plane* translation (MP view) in mm. It is described as • Anterior - or - • Posterior
8	Insert *axial translation* (Axial view) in mm as • Short, used when the moving bone segment is translated (compressed) towards the reference bone segment - or - • Long, used when the moving bone segment is translated (distracted) away the reference bone segment *Bone length* is a clinical paramater indicating limb length discrepancy relative to the contralateral limb. • Short - or - • Long Depending on the relevant amount of bone length discrepancy in mm.
9	Click [Update Views] button at any time to refresh the display according to the parameters entered
10	These are three diagrams in the software. AP view: corresponding to the AP X-ray of the limb ML view: representing the ML X-ray of the limb Axial view: representing the view looking either up or down the limb from the reference segment
11	Click on [Previous] button to return to the previous tab [Case Data]
12	Click on [Next] button to move to the next tab [Frame Parameters]

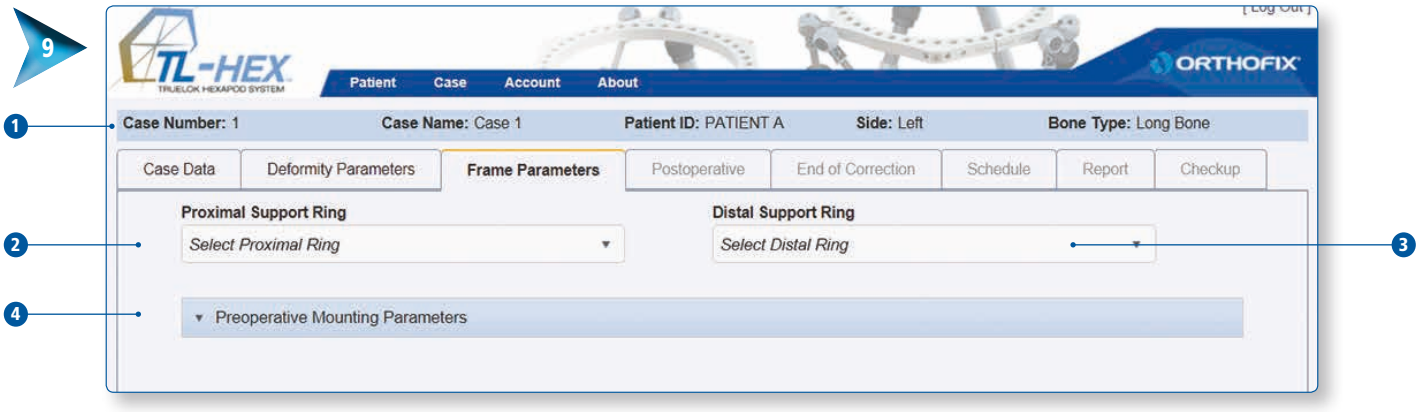
9
TL-HEX
TRUELOK HEXAPOD SYSTEM
Patient
Case
Account
About
ORTHOFIX
1
Case Number: 1
Case Name: Case 1
Patient ID: PATIENT A
Side: Left
Bone Type: Long Bone
Case Data
Deformity Parameters
Frame Parameters
Postoperative
End of Correction
Schedule
Report
Checkup
Proximal Support Ring
2
Select Proximal Ring
Distal Support Ring
Select Distal Ring
3
4
Preoperative Mounting Parameters

9. Frame Parameters			
	Description		
1	Summary of Case Data provided in the Case Data tab		
External Supports specification			
	Ring Type available	Ring Size available	Footplate Size available
	Full Ring	100mm	120mm
	Full Ring (5/8 plus 3/8)	120mm	140mm
	5/8 Open Anteriorly Ring	140mm	160mm
	5/8 Open Medially Ring	160mm	180mm
	5/8 Open Posteriorly Ring	180mm	220mm
	Footplate	200mm	
		220mm	
		240mm	
		280mm	
		300mm	
2	Select proximal support ring type and size from the drop-down selectors		
3	Select distal support ring type and size from the drop-down selectors		
4	Optionally expand Preoperative Mounting Parameters bar to do a pre-planning of the case (see screen N°. 9.1 for details)		

9.1
6
9
8
TL-HEX
TRUELOK HEXAPOD SYSTEM
ORTHOFIX
Patient
Case
Account
About
Case Number: 1
Case Name: Case 1
Patient ID: PATIENT A
Side: Left
Bone Type: Long Bone
Case Data
Deformity Parameters
Frame Parameters
Postoperative
End of Correction
Schedule
Report
Checkup
Proximal Support Ring
Select Proximal Ring
Distal Support Ring
Select Distal Ring
Preoperative Mounting Parameters
Reference Ring AP Translation (mm)
Medial
Lateral
Reference Ring ML Translation (mm)
Anterior
Posterior
Reference Ring Position Relative To
Deformity Apex
Osteotomy/Fracture Level
Reference Ring Position (mm)
Proximal
Distal
Reference Ring Frame Rotation (deg)
Second Ring Position (mm)
Update Views
AP view
ML view
Axial view
Total
Strut 1 (mm): 166
Strut 2 (mm): 132
Strut 3 (mm): 95
Strut 4 (mm): 88
Strut 5 (mm): 111
Strut 6 (mm): 154
Size
Medium
Medium
Short
Ultra Short
Short
Medium
Acute
18
0
3
28
15
6
Gradual
1
17
14
13
11
1
Privacy Policy
EULA
Cookies
Contact Us
Instructions for Use
5
7
10
13
14
11
12

9.1 Preoperative Mounting Parameters Section

PREOPERATIVE MOUNTING PARAMETERS SECTION - optional. The default assumption is that both proximal and distal external supports are perpendicular to the corresponding bone segment axis and located at 50mm distance from the point of interest.

	Description
5	Adjust the position of the reference ring in the coronal plane (AP translation) in mm • Medial - or - • Lateral
6	Adjust the position of the reference ring in the sagittal plane (ML translation) in mm • Anterior - or - • Posterior
7	Adjust the reference ring position, in the axial direction in mm, described as • Proximal - or - • Distal Adjust the moving ring (second ring) position in mm
8	Determine the point of interest for the reference ring position Relative to Deformity Apex - or - Relative to Osteotomy/Fracture Level Refer to Fig. 2 for the description of the reference ring position relative to deformity apex (a) or osteotomy/fracture level (b) 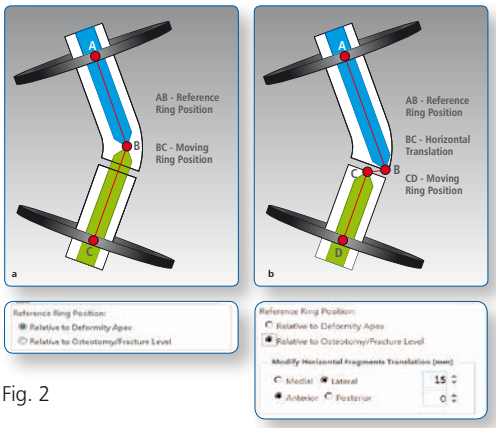 Fig. 2 If the AP or ML view translation was entered into the deformity parameters section, the osteotomy/fracture level is automatically chosen as point of interest
9	Frame Rotation field with the relevant read-only value. The software will automatically change the orientation offset of the 5/8 ring
10	Click [Update Views] button, after entering the mounting parameters, will reveal the preassembled frame construct and render a set of strut lenghts that will result in the required frame
11	These are the three diagrams in the software. AP view: corresponding to the AP X-ray of the limb ML view: representing the ML X-ray of the limb Axial view: representing the view looking either up or down the limb from the reference segment
12	This area shows the strut mounting parameters for all six struts. Details for each strut are described in three fields: • [Size]: Strut size (ultra short, short, medium, long) • [Acute]: Acute length for the strut in mm, which is read off the scale relative to the acute length orange mark • [Gradual]: Gradual length for the strut in mm, which is read off the scale relative to the gradual length green mark
13	Click on [Previous] button to return to the previous tab [Deformity Parameters]
14	Click on [Next] button to move to the next tab [Postoperative]

10
TL-HEX
TRUELOK HEXAPOD SYSTEM
Patient
Case
Account
About
ORTHOFIX
1
Case Number: 1
Case Name: Case 1
Patient ID: PATIENT A
Side: Left
Bone Type: Long Bone
Case Data
Deformity Parameters
Frame Parameters
Postoperative
End of Correction
Schedule
Report
Checkup
2
Reference Ring AP Plane Angle (deg)
0
Medial Side Down
Medial Side Up
3
Reference Ring ML Plane Angle (deg)
0
Anterior Side Down
Anterior Side Up
8
Reference Ring Position Relative To
Deformity Apex
Osteotomy/Fracture Level
4
Reference Ring AP Translation (mm)
0
Medial
Lateral
5
Reference Ring ML Translation (mm)
25
Anterior
Posterior
6
Reference Ring Position (mm)
100
Proximal
Distal
7
Reference Ring Frame Rotation (deg)
0
External
Internal
9
Update Views
AP view
ML view
Axial view
10
13
14
11
Apply First Strut To All Struts
12
Total
Size
Acute
Gradual
Strut 1 (mm): 254
Strut 2 (mm): 209
Strut 3 (mm): 162
Strut 4 (mm): 149
Strut 5 (mm): 179
Strut 6 (mm): 239
Long
Long
Long
Medium
Long
Long
17
50
3
34
20
2
1
79
79
34
79
1
Privacy Policy
EULA
Cookies
Contact Us
Instructions for Use

10. Postoperative	
	Description
1	Summary of Case Data provided in the Case Data tab
Reference Ring Position	Refer to Fig. 3 to determine the reference ring angulation, translation and rotation parameters in AP view (a), ML view (b) and axial view (c). 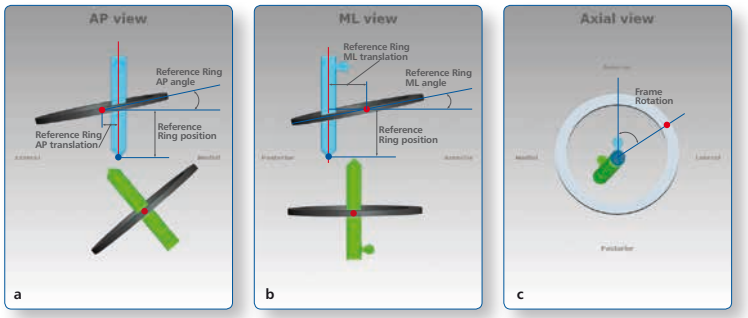 Fig. 3
2	Enter the reference ring angle on the AP view in degrees as the angle between the projection of the ring and the axis of the bone segment with the medial side of the ring. • Medial side up - or - • Medial side down
3	Enter the reference ring angle on the ML view in degrees as the angle between the projection of the ring and the axis of bone segment with the anterior side of the ring. • Anterior side up - or - • Anterior side down
4	Adjust/Enter the position of the reference ring in the coronal plane (AP translation) in mm as translation of the center of the reference ring in relation to the longitudinal axis of the reference bone segment • Medial - or - • Lateral
5	Adjust/Enter the position of the reference ring in the sagittal plane (ML translation) in mm as translation of the center of the reference ring in relation to the longitudinal axis of the reference bone segment • Anterior - or - • Posterior
6	Adjust/Enter the reference ring position, in the axial direction in mm, described as the translation of the reference ring proximal/distal along the longitudinal axis of the reference bone segment • Proximal - or - • Distal
7	Specify the frame rotation relative to the longitudinal axis of the reference bone segment in degrees on the axial view, described as • External rotation - or - • Internal rotation
8	Determine the point of interest for the reference ring position. See Screen 9.1 - Reference 8 for more details. • Relative to Deformity Apex - or - • Relative to Osteotomy/Fracture Level
9	Click [Update Views] button at any time to refresh the display according to the parameters entered. At this point, the software will generate diagrammatic models that reflect the bone deformity and frame position on the X-ray. In case of discrepancy, the surgeon should go back and the check all the variables before proceeding to the next steps.
10	These are the three diagrams in the software. AP view: corresponding to the AP X-ray of the limb ML view: representing the ML X-ray of the limb Axial view: representing the view looking either up or down the limb from the reference segment
11	Click [Apply First Strut To All Struts] to apply the size, acute and gradual values of the first strut to all the others
12	This area shows the strut mounting parameters for all six struts. Details for each strut are described in three fields: • [Size]: Strut size (ultra short, short, medium, long) • [Acute]: Acute length for the strut in mm, which is read off the scale relative to the acute length orange mark • [Gradual]: Gradual length for the strut in mm, which is read of the scale relative to the gradual length green mark Confirm or adjust the data if necessary. Correct any additional errors prior to proceeding with the next steps. An error is highlighted in red and the strut size and length should be corrected.
13	Click on [Previous] button to return to the previous tab [Frame Parameters]
14	Click on [Next] button to move to the next tab [End of Correction]

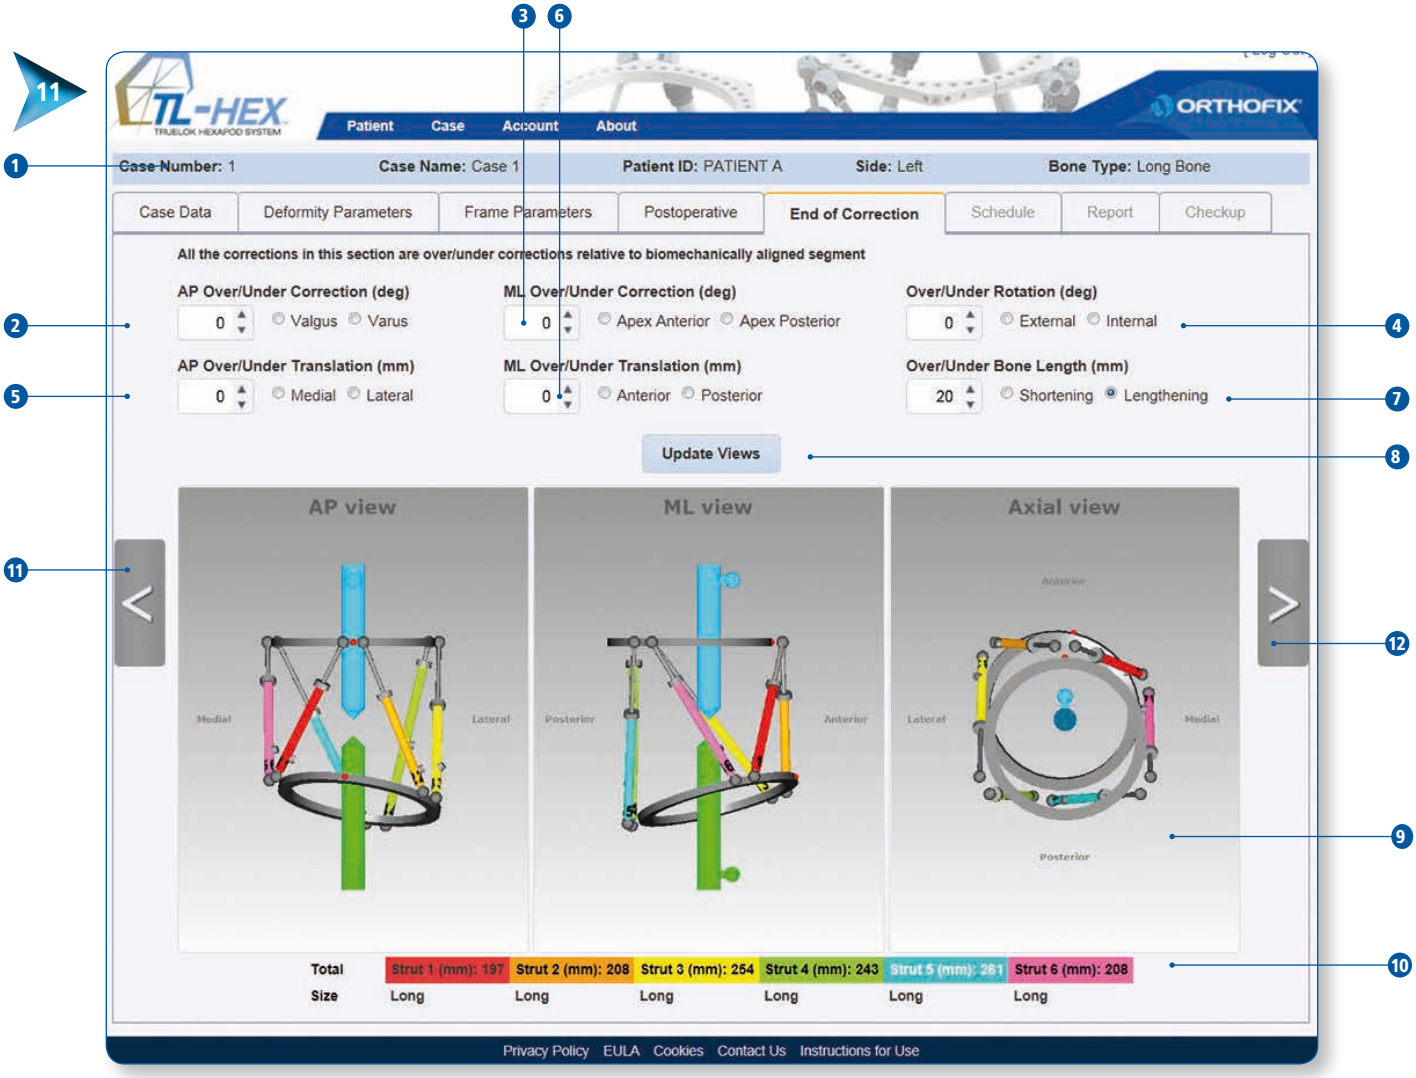
11
3
6
1
2
4
5
7
8
11
12
9
10
TL-HEX
TRUELOK HEXAPOD SYSTEM
Patient
Case
Account
About
ORTHOFIX
Case Number: 1
Case Name: Case 1
Patient ID: PATIENT A
Side: Left
Bone Type: Long Bone
Case Data
Deformity Parameters
Frame Parameters
Postoperative
End of Correction
Schedule
Report
Checkup
All the corrections in this section are over/under corrections relative to biomechanically aligned segment
AP Over/Under Correction (deg)
0
Valgus
Varus
ML Over/Under Correction (deg)
0
Apex Anterior
Apex Posterior
Over/Under Rotation (deg)
0
External
Internal
AP Over/Under Translation (mm)
0
Medial
Lateral
ML Over/Under Translation (mm)
0
Anterior
Posterior
Over/Under Bone Length (mm)
20
Shortening
Lengthening
Update Views
AP view
ML view
Axial view
Medial
Lateral
Posterior
Anterior
Total
Size
Strut 1 (mm): 197
Strut 2 (mm): 208
Strut 3 (mm): 254
Strut 4 (mm): 243
Strut 5 (mm): 261
Strut 6 (mm): 208
Long
Privacy Policy
EULA
Cookies
Contact Us
Instructions for Use

11. End of Correction	
	Description
1	Summary of Case Data provided in the Case Data tab
The software assumes that, at the end of the treatment, the bone segments should be in perfect alignment or, in case of a foot case, the segments should be perfectly perpendicular. However, surgeon could override the default position as desired	
ANGULATION	
2	Override (Over/Under) AP correction in degrees. This can be either • Valgus - or - • Varus
3	Override (Over/Under) ML correction in degrees. This can be either • Apex anterior - or - • Apex posterior
4	Override (Over/Under) rotation in degree . It is described as • External - or - • Internal
TRANSLATION	
5	Override (Over/Under) AP translation in mm. It is described as • Medial - or - • Lateral
6	Override (Over/Under) ML translation in mm. It is described as • Anterior - or - • Posterior
7	Select the bone length • Shortening - or - • Lengthening
8	Click [Update Views] button at any time to refresh the display according to the parameters entered and check the bottom of the screen for struts that are out of range.
9	These are the three diagrams in the software. AP view: corresponding to the AP X-ray of the limb ML view: representing the ML X-ray of the limb Axial view: representing the view looking either up or down the limb from the reference segment
10	This area shows the strut size for all six struts.
11	Click on [Previous] button to return to the previous tab [Postoperative]
12	Click on [Next] button to move to the next tab [Schedule]

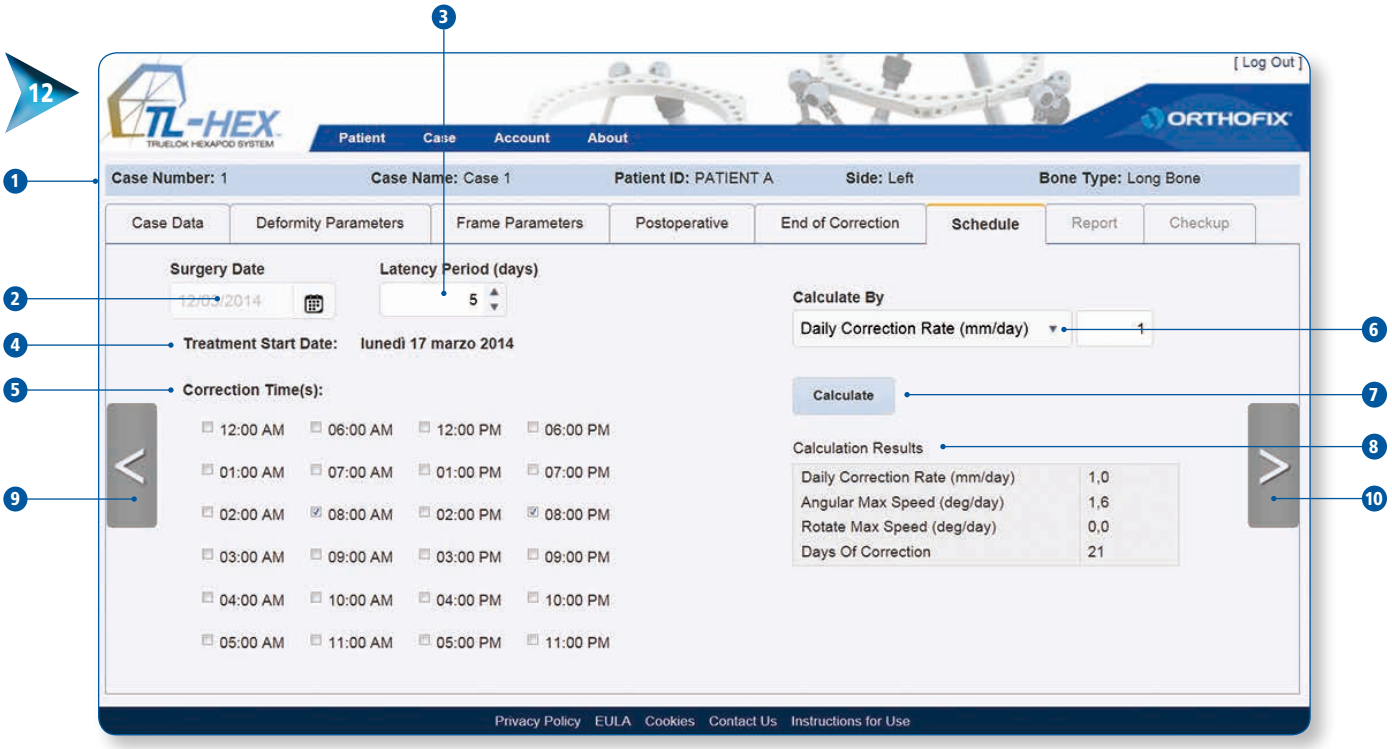
12
3
[Log Out]
TL-HEX
TRUELOK HEXAPOD SYSTEM
Patient
Case
Account
About
ORTHOFIX
1
Case Number: 1
Case Name: Case 1
Patient ID: PATIENT A
Side: Left
Bone Type: Long Bone
Case Data
Deformity Parameters
Frame Parameters
Postoperative
End of Correction
Schedule
Report
Checkup
Surgery Date
2
Latency Period (days)
5
Calculate By
Daily Correction Rate (mm/day)
1
6
4
Treatment Start Date:
lunedì 17 marzo 2014
5
Correction Time(s):
Calculate
7
12:00 AM
06:00 AM
12:00 PM
06:00 PM
01:00 AM
07:00 AM
01:00 PM
07:00 PM
02:00 AM
08:00 AM
02:00 PM
08:00 PM
03:00 AM
09:00 AM
03:00 PM
09:00 PM
04:00 AM
10:00 AM
04:00 PM
10:00 PM
05:00 AM
11:00 AM
05:00 PM
11:00 PM
Calculation Results
8
Daily Correction Rate (mm/day) 1,0
Angular Max Speed (deg/day) 1,6
Rotate Max Speed (deg/day) 0,0
Days Of Correction 21
9
10
Privacy Policy
EULA
Cookies
Contact Us
Instructions for Use

12. Schedule	
	Description
1	Summary of Case Data provided in the Case Data tab
2	Indicate the Surgery date
3	Indicate the latency period in days. By default it is 5 days
4	The software determines the treatment start date considering surgery date plus latency period
5	Indicate up to 4 correction time/s to have the prescription calculated for one or more frame adjustments per treatment day
6	Specify a calculating rate: - Daily Correction Rate: maximum rate of the bone segment translation (mm/day) - Angular Max Speed: maximum rate of the bone segment rotation (degrees/day) - Rotate Max Speed: maximum rate of the bone segment angular correction (degrees/day) - Days of Correction
7	Click [Calculate] to calculate the speed of correction after having selected one of the rate above. (It is necessary to enter at least one value in the "Calculate By" box and "Correction time(s)" box prior to click)
8	Calculation Results box shows the resulting values of calculation for each rate, automatically calculated using also decimal
9	Click [Previous] button to return to the previous tab [End of Correction]
10	Click [Next] button to move to the next tab [Report]

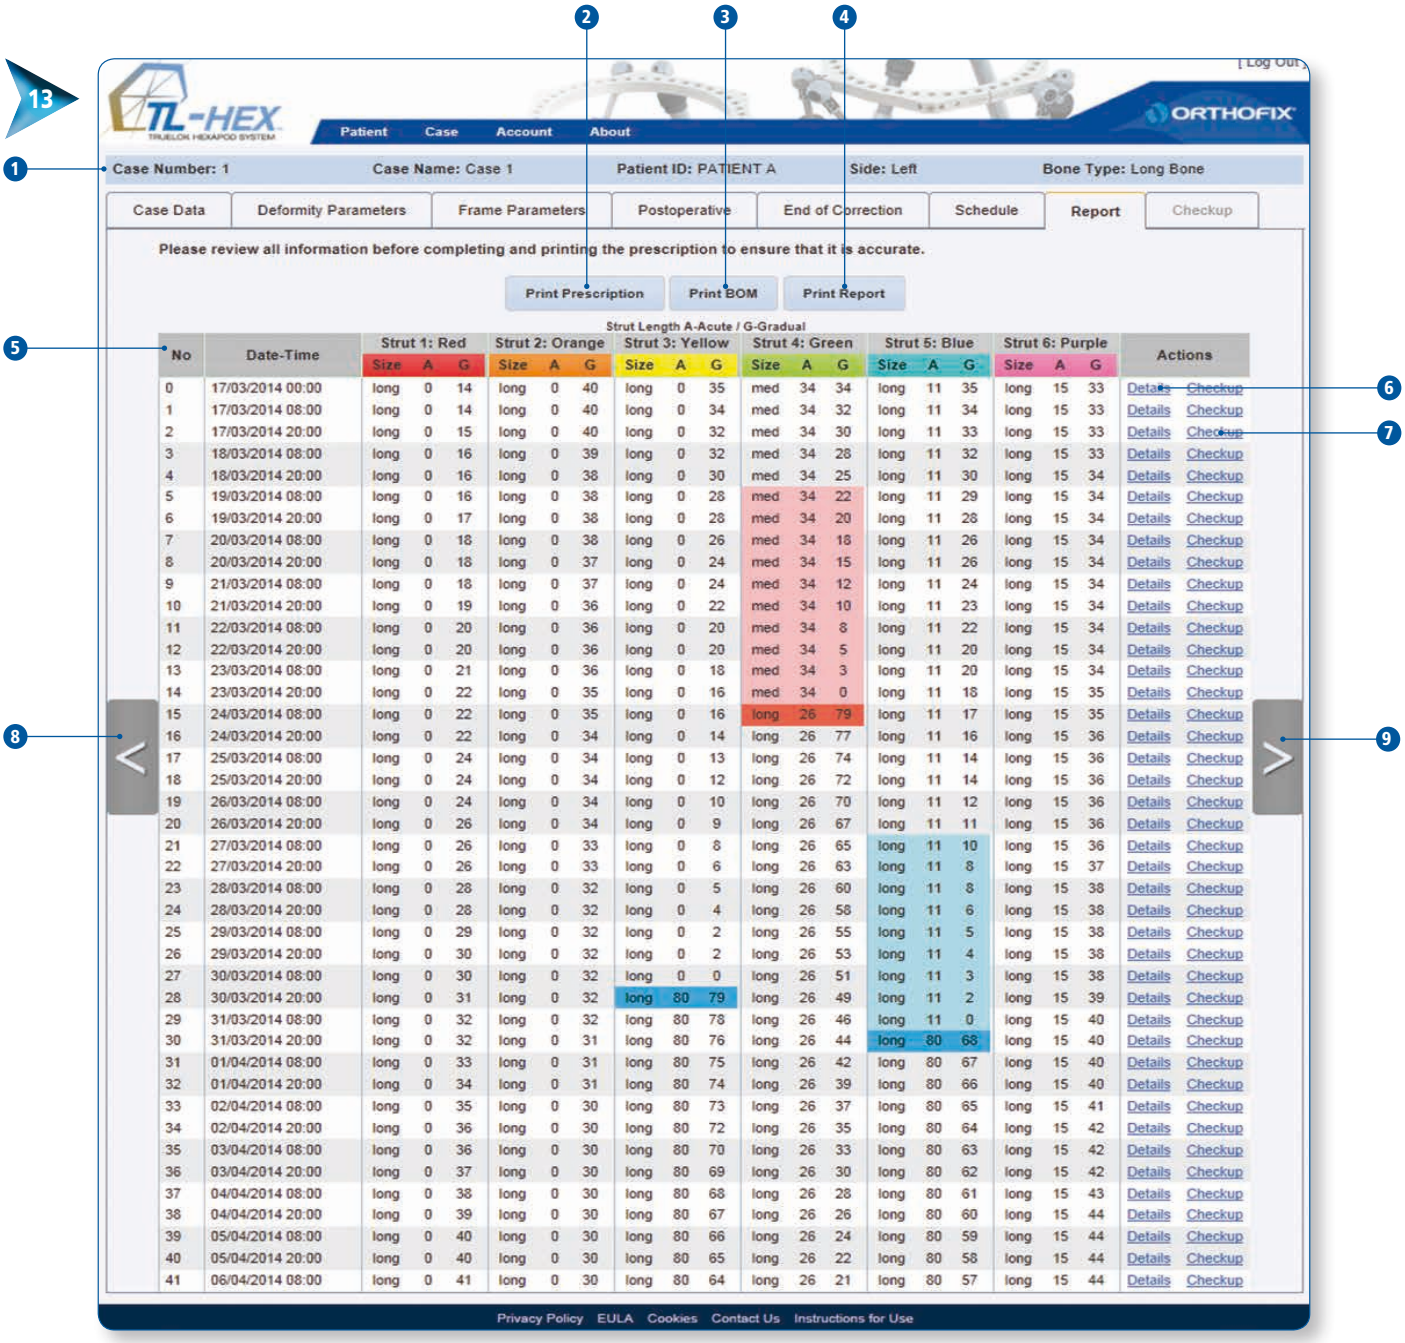

No	Date-Time	Strut 1: Red			Strut 2: Orange			Strut 3: Yellow			Strut 4: Green			Strut 5: Blue			Strut 6: Purple		
		Size	A	G	Size	A	G	Size	A	G	Size	A	G	Size	A	G	Size	A	G
0	17/03/2014 00:00	long	0	14	long	0	40	long	0	35	med	34	34	long	11	35	long	15	33
1	17/03/2014 08:00	long	0	14	long	0	40	long	0	34	med	34	32	long	11	34	long	15	33
2	17/03/2014 20:00	long	0	15	long	0	40	long	0	32	med	34	30	long	11	33	long	15	33
3	18/03/2014 08:00	long	0	16	long	0	39	long	0	32	med	34	28	long	11	32	long	15	33
4	18/03/2014 20:00	long	0	16	long	0	38	long	0	30	med	34	25	long	11	30	long	15	34
5	19/03/2014 08:00	long	0	16	long	0	38	long	0	28	med	34	22	long	11	29	long	15	34
6	19/03/2014 20:00	long	0	17	long	0	38	long	0	28	med	34	20	long	11	28	long	15	34
7	20/03/2014 08:00	long	0	18	long	0	38	long	0	26	med	34	18	long	11	26	long	15	34
8	20/03/2014 20:00	long	0	18	long	0	37	long	0	24	med	34	15	long	11	26	long	15	34
9	21/03/2014 08:00	long	0	18	long	0	37	long	0	24	med	34	12	long	11	24	long	15	34
10	21/03/2014 20:00	long	0	19	long	0	36	long	0	22	med	34	10	long	11	23	long	15	34
11	22/03/2014 08:00	long	0	20	long	0	36	long	0	20	med	34	8	long	11	22	long	15	34
12	22/03/2014 20:00	long	0	20	long	0	36	long	0	20	med	34	5	long	11	20	long	15	34
13	23/03/2014 08:00	long	0	21	long	0	36	long	0	18	med	34	3	long	11	20	long	15	34
14	23/03/2014 20:00	long	0	22	long	0	35	long	0	16	med	34	0	long	11	18	long	15	35
15	24/03/2014 08:00	long	0	22	long	0	35	long	0	16	long	26	79	long	11	17	long	15	35
16	24/03/2014 20:00	long	0	22	long	0	34	long	0	14	long	26	77	long	11	16	long	15	36
17	25/03/2014 08:00	long	0	24	long	0	34	long	0	13	long	26	74	long	11	14	long	15	36
18	25/03/2014 20:00	long	0	24	long	0	34	long	0	12	long	26	72	long	11	14	long	15	36
19	26/03/2014 08:00	long	0	24	long	0	34	long	0	10	long	26	70	long	11	12	long	15	36
20	26/03/2014 20:00	long	0	26	long	0	34	long	0	9	long	26	67	long	11	11	long	15	36
21	27/03/2014 08:00	long	0	26	long	0	33	long	0	8	long	26	65	long	11	10	long	15	36
22	27/03/2014 20:00	long	0	26	long	0	33	long	0	6	long	26	63	long	11	8	long	15	37
23	28/03/2014 08:00	long	0	28	long	0	32	long	0	5	long	26	60	long	11	8	long	15	38
24	28/03/2014 20:00	long	0	28	long	0	32	long	0	4	long	26	58	long	11	6	long	15	38
25	29/03/2014 08:00	long	0	29	long	0	32	long	0	2	long	26	55	long	11	5	long	15	38
26	29/03/2014 20:00	long	0	30	long	0	32	long	0	2	long	26	53	long	11	4	long	15	38
27	30/03/2014 08:00	long	0	30	long	0	32	long	0	0	long	26	51	long	11	3	long	15	38
28	30/03/2014 20:00	long	0	31	long	0	32	long	80	79	long	26	49	long	11	2	long	15	39
29	31/03/2014 08:00	long	0	32	long	0	32	long	80	78	long	26	46	long	11	0	long	15	40
30	31/03/2014 20:00	long	0	32	long	0	31	long	80	76	long	26	44	long	80	68	long	15	40
31	01/04/2014 08:00	long	0	33	long	0	31	long	80	75	long	26	42	long	80	67	long	15	40
32	01/04/2014 20:00	long	0	34	long	0	31	long	80	74	long	26	39	long	80	66	long	15	40
33	02/04/2014 08:00	long	0	35	long	0	30	long	80	73	long	26	37	long	80	65	long	15	41
34	02/04/2014 20:00	long	0	36	long	0	30	long	80	72	long	26	35	long	80	64	long	15	42
35	03/04/2014 08:00	long	0	36	long	0	30	long	80	70	long	26	33	long	80	63	long	15	42
36	03/04/2014 20:00	long	0	37	long	0	30	long	80	69	long	26	30	long	80	62	long	15	42
37	04/04/2014 08:00	long	0	38	long	0	30	long	80	68	long	26	28	long	80	61	long	15	43
38	04/04/2014 20:00	long	0	39	long	0	30	long	80	67	long	26	26	long	80	60	long	15	44
39	05/04/2014 08:00	long	0	40	long	0	30	long	80	66	long	26	24	long	80	59	long	15	44
40	05/04/2014 20:00	long	0	40	long	0	30	long	80	65	long	26	22	long	80	58	long	15	44
41	06/04/2014 08:00	long	0	41	long	0	30	long	80	64	long	26	21	long	80	57	long	15	44

13. Report	
	Description
1	Summary of Case Data provided in the Case Data tab
2	Click [Print Prescription] to generate a prescription in .pdf format. This document can be saved for the record and printed as hard copy to be issued to the patient. (see screen N°. 13.1 for details)
3	Click [Print BOM] to generate a bill of materials in .pdf format. This document lists the materials that only cover the TL-HEX components needed for the treatment. (see screen N°. 13.2 for details)
4	Click [Print Report] to generate a report in .pdf format. This document can be saved for the record or printed as hard copy. (see screen N°. 13.3 for details)
5	The table report provides: - number of line - date and time of the treatment for each line - information, for each strut and line, about size, acute and gradual adjustments in millimeters - actions that can be made on each line The report and prescription rows will be highlighted when strut readjustments (shaded blue) or exchanges (shaded red) are required. The rows of the lighter shading indicate the allowable range of days that is suitable for the readjustment/excahnge; the heavier shaded row indicates the last possible day for the strut change.
6	Click [Details] of a row to view three views of the deformity and the frame for the corresponding date/time of the treatment and the related struts values.
7	Click [Checkup] to launch the Checkup for the selected day and time
8	Click on [Previous] button to return to the previous tab [Schedule]
9	Click on [Next] button to move to the next tab [Checkup]

13.1

Dr. test2 account2
Hospital name
test address
City State Test 012344
012345675

Print Date: venerdì 18 luglio 2014

Page 1

Case Number: Test BL_AT
Case Name: TestBL-AT
Patient ID: 12
Side: Left
Bone Type: Long Bone

Notes:

notes for patient

		Strut Adjustments in 'CLICKS'						Strut Reference Length					
		RED	ORANGE	YELLOW	GREEN	BLUE	PURPLE	RED	ORANGE	YELLOW	GREEN	BLUE	PURPLE
No	Date-Time	Strut1	Strut2	Strut3	Strut4	Strut5	Strut6	Strut1	Strut2	Strut3	Strut4	Strut5	Strut6
0	07/07/2014 00:00	0	0	0	0	0	0	14	1	14	1	14	1
1	07/07/2014 14:00	+3	-2	+3	-2	+3	-2	12	2	12	2	12	2
2	08/07/2014 14:00	+4	-3	+4	-3	+4	-3	10	4	10	4	10	4
3	09/07/2014 14:00	+4	-3	+4	-3	+4	-3	8	5	8	5	8	5
4	10/07/2014 14:00	+5	-3	+5	-3	+5	-3	6	6	6	6	6	6
5	11/07/2014 14:00	+5	-3	+5	-3	+5	-3	4	8	4	8	4	8
6	12/07/2014 14:00	+5	-3	+5	-3	+5	-3	1	10	1	10	1	10
7	13/07/2014 14:00	0	-3	0	-3	0	-3	34	11	34	11	34	11
8	14/07/2014 14:00	+5	-3	+5	-3	+5	-3	32	12	32	12	32	12
9	15/07/2014 14:00	+5	-3	+5	-3	+5	-3	29	14	29	14	29	14
10	16/07/2014 14:00	+5	-3	+5	-3	+5	-3	27	16	27	16	27	16
11	17/07/2014 14:00	+5	-3	+5	-3	+5	-3	24	17	24	17	24	17
12	18/07/2014 14:00	+6	-3	+6	-3	+6	-3	21	18	21	18	21	18
13	19/07/2014 14:00	+5	-3	+5	-3	+5	-3	19	20	19	20	19	20
14	20/07/2014 14:00	+5	-2	+5	-2	+5	-2	16	21	16	21	16	21
15	21/07/2014 14:00	+6	-3	+6	-3	+6	-3	13	22	13	22	13	22
16	22/07/2014 14:00	+5	-2	+5	-2	+5	-2	11	24	11	24	11	24
17	23/07/2014 14:00	+5	-3	+5	-3	+5	-3	8	25	8	25	8	25
18	24/07/2014 14:00	+6	-2	+6	-2	+6	-2	5	26	5	26	5	26
19	25/07/2014 14:00	+5	-2	+5	-2	+5	-2	3	27	3	27	3	27

13.2

Case Number: Test BL_AT
Case Name: TestBL-AT
Patient ID: 12
Side: Left
Bone Type: Long Bone

BOM Print Date: venerdì 18 luglio 2014
Page 1

Item	Description	QTY Reqd	Item Number
Strut	Short	3	50-10200
Strut	Medium	6	50-10300
Distal Ring	Full Ring 180mm	1	56-20040
Proximal Ring	Full Ring 180mm	1	56-20040

The listed materials only cover the TL-HEX components needed for the treatment. This includes rings, foot plates, and struts.

13.1 Prescription PDF	
	Description
1	Prescription Preferences are presented here. The default is the registration address but it is possible to enter and choose among up to 4 different addresses
2	Information about date of print and case details are presented here
3	Notes entered on the prescription preferences notes or, if this last one are not present, on add new patient screen are presented here
4	[Strut Adjustments in 'CLICKS']Represent the adjustment for each strut by number of clicks (1/2 rotation of the strut adjustment knob). It can be * positive (if strut length increases) - or- *negative (if strut length decreases) [Strut Reference Length] Represent the gradual adjustment scale value in millimeters as reference for each strut

13.2 BOM PDF	
	Description
1	The information about the case is presented here along with the printing date
2	The table summarize the type, quantity and number of the items needed during the treatment period. **The listed materials only cover the TL-HEX components needed for the treatment. This includes rings, foot plates and struts.**

13.3

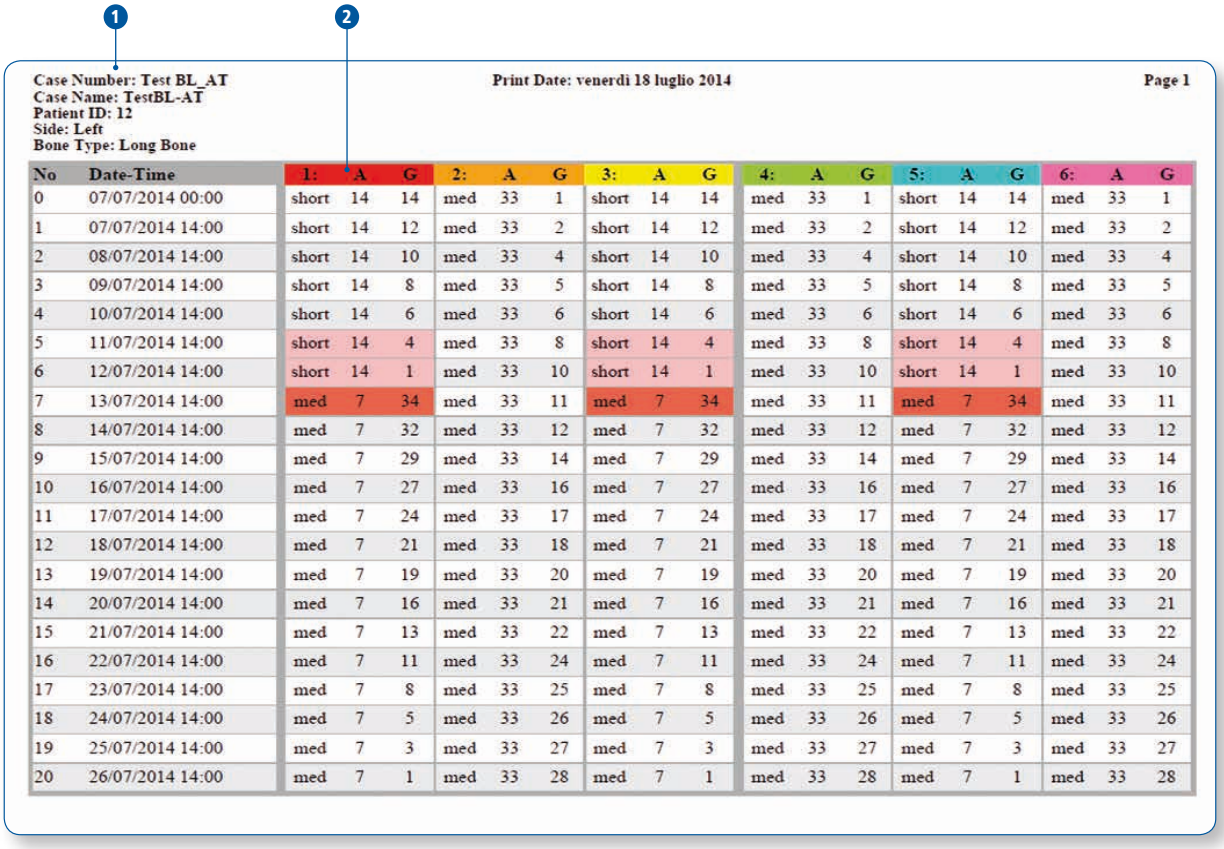

Case Number: Test BL_AT
Case Name: TestBL-AT
Patient ID: 12
Side: Left
Bone Type: Long Bone

Print Date: venerdì 18 luglio 2014

Page 1

No	Date-Time	1:	A	G	2:	A	G	3:	A	G	4:	A	G	5:	A	G	6:	A	G
0	07/07/2014 00:00	short	14	14	med	33	1	short	14	14	med	33	1	short	14	14	med	33	1
1	07/07/2014 14:00	short	14	12	med	33	2	short	14	12	med	33	2	short	14	12	med	33	2
2	08/07/2014 14:00	short	14	10	med	33	4	short	14	10	med	33	4	short	14	10	med	33	4
3	09/07/2014 14:00	short	14	8	med	33	5	short	14	8	med	33	5	short	14	8	med	33	5
4	10/07/2014 14:00	short	14	6	med	33	6	short	14	6	med	33	6	short	14	6	med	33	6
5	11/07/2014 14:00	short	14	4	med	33	8	short	14	4	med	33	8	short	14	4	med	33	8
6	12/07/2014 14:00	short	14	1	med	33	10	short	14	1	med	33	10	short	14	1	med	33	10
7	13/07/2014 14:00	med	7	34	med	33	11	med	7	34	med	33	11	med	7	34	med	33	11
8	14/07/2014 14:00	med	7	32	med	33	12	med	7	32	med	33	12	med	7	32	med	33	12
9	15/07/2014 14:00	med	7	29	med	33	14	med	7	29	med	33	14	med	7	29	med	33	14
10	16/07/2014 14:00	med	7	27	med	33	16	med	7	27	med	33	16	med	7	27	med	33	16
11	17/07/2014 14:00	med	7	24	med	33	17	med	7	24	med	33	17	med	7	24	med	33	17
12	18/07/2014 14:00	med	7	21	med	33	18	med	7	21	med	33	18	med	7	21	med	33	18
13	19/07/2014 14:00	med	7	19	med	33	20	med	7	19	med	33	20	med	7	19	med	33	20
14	20/07/2014 14:00	med	7	16	med	33	21	med	7	16	med	33	21	med	7	16	med	33	21
15	21/07/2014 14:00	med	7	13	med	33	22	med	7	13	med	33	22	med	7	13	med	33	22
16	22/07/2014 14:00	med	7	11	med	33	24	med	7	11	med	33	24	med	7	11	med	33	24
17	23/07/2014 14:00	med	7	8	med	33	25	med	7	8	med	33	25	med	7	8	med	33	25
18	24/07/2014 14:00	med	7	5	med	33	26	med	7	5	med	33	26	med	7	5	med	33	26
19	25/07/2014 14:00	med	7	3	med	33	27	med	7	3	med	33	27	med	7	3	med	33	27
20	26/07/2014 14:00	med	7	1	med	33	28	med	7	1	med	33	28	med	7	1	med	33	28

13.3 Report PDF	
	Description
1	Information about date of print and case details are presented here
2	Provides a more detailed prescription. In addition to the patient prescription it includes • Strut size • Acute adjustment in millimeters • Gradual adjustment in millimeters for each strut

14
TL-HEX
TRUELOK HEXAPOD SYSTEM
Patient
Case
Account
About
ORTHOFIX
1
Case Number: 1
Case Name: Case 1
Patient ID: PATIENT A
Side: Left
Bone Type: Long Bone
Case Data
Deformity Parameters
Frame Parameters
Postoperative
End of Correction
Schedule
Report
Checkup
2
Treatment Date
17/03/2014
Displaying Report line number 0 based on treatment range of: 17/03/2014 - 06/04/2014
AP view
ML view
Axial view
3
8
AP Angle (deg): 25 Valgus
AP Translation (mm): 0
ML Angle (deg): 25 ApexAnterior
ML Translation (mm): 0
Rotation (deg): 0
Axial Translation (mm): 0
4
Total
Strut 1 (mm): 224
Strut 2 (mm): 198
Strut 3 (mm): 203
Strut 4 (mm): 149
Strut 5 (mm): 214
Strut 6 (mm): 220
Size
Long
Long
Long
Medium
Long
Long
Acute
0
0
0
34
11
15
Gradual
14
40
35
34
35
33
To Create New Case
5
New Case Number:
CopyOf_1
6
New Case Name:
Case 1_Copied on 13/03/2014
7
Create New Case
Privacy Policy
EULA
Cookies
Contact Us
Instructions for Use

14. Checkup	
	Description
1	Summary of Case Data provided in the Case Data tab
Provides the position of the bone segments and the frame with corresponding strut adjustment values at any particular day of treatment (deformity correction)	
2	Select the treatment date. As default, the screen shows the data for the current day during the treatment period
3	These are the three diagrams in the software considering the deformity and the frame for the corresponding day/time of the prescription. AP view: corresponding to the AP X-ray of the limb ML view: representing the ML X-ray of the limb Axial view: representing the view looking either up or down the limb from the reference segment All the deformity and frame parameters are transferred from the previous case at the date of check-up
4	These are the values of the struts (size, acute, gradual) for the corresponding day/time of the prescription (treatment date)
5	Enter new case detail - Case Number
6	Enter new case detail - Case Name
7	Click [Create New Case] to open a new Case data screen for the newly generated case (the deformity/frame parameters of the selected treatment date will be copied in the new case)
8	Click on [Previous] button to return to the previous tab [Report]
Select the treatment date. Default: - If current day is within the treatment rage the checkup date displayed is the current one - If treatment has not yet started the first day of treatment is presented as default and a message is displayed showing the allowed treatment range - If treatment has been completed the last day of treatment is presented as default and a message is displayed showing the allowed treatment range	

15

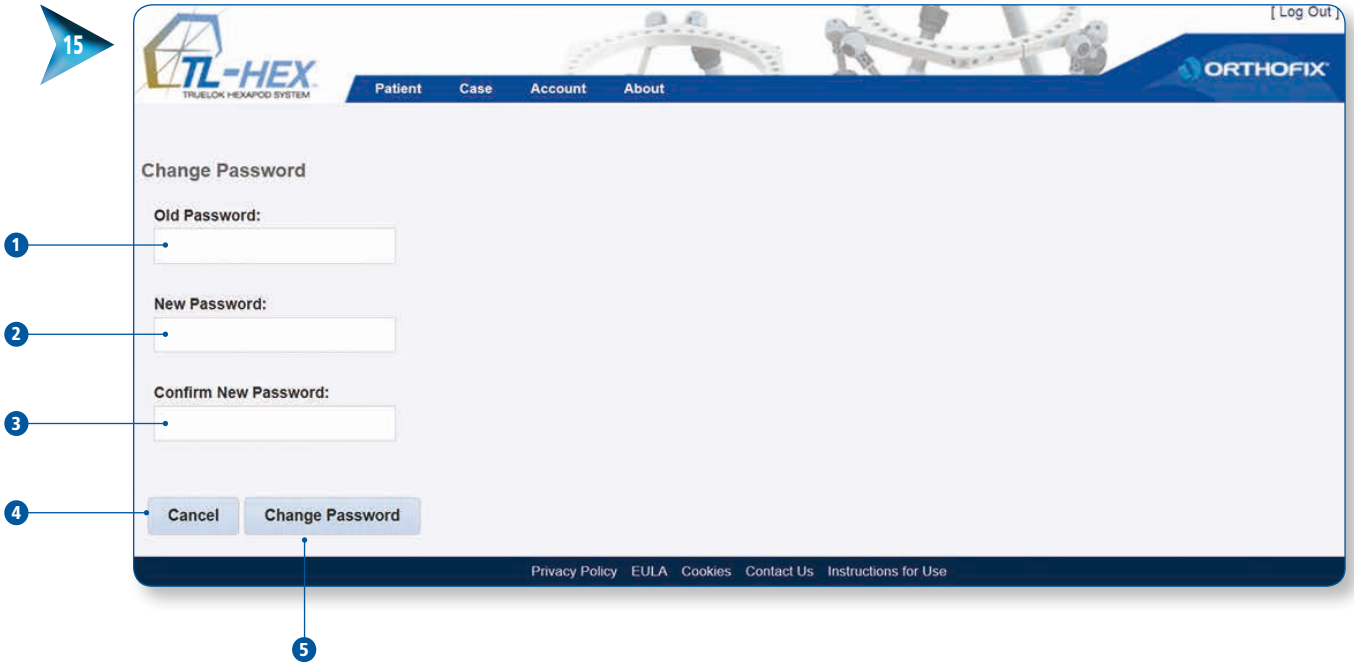
[Log Out]
TL-HEX
TRUELOK HEXAPOD SYSTEM
Patient
Case
Account
About
ORTHOFIX
Change Password
Old Password:
New Password:
Confirm New Password:
Cancel
Change Password
Privacy Policy
EULA
Cookies
Contact Us
Instructions for Use
1
2
3
4
5

16

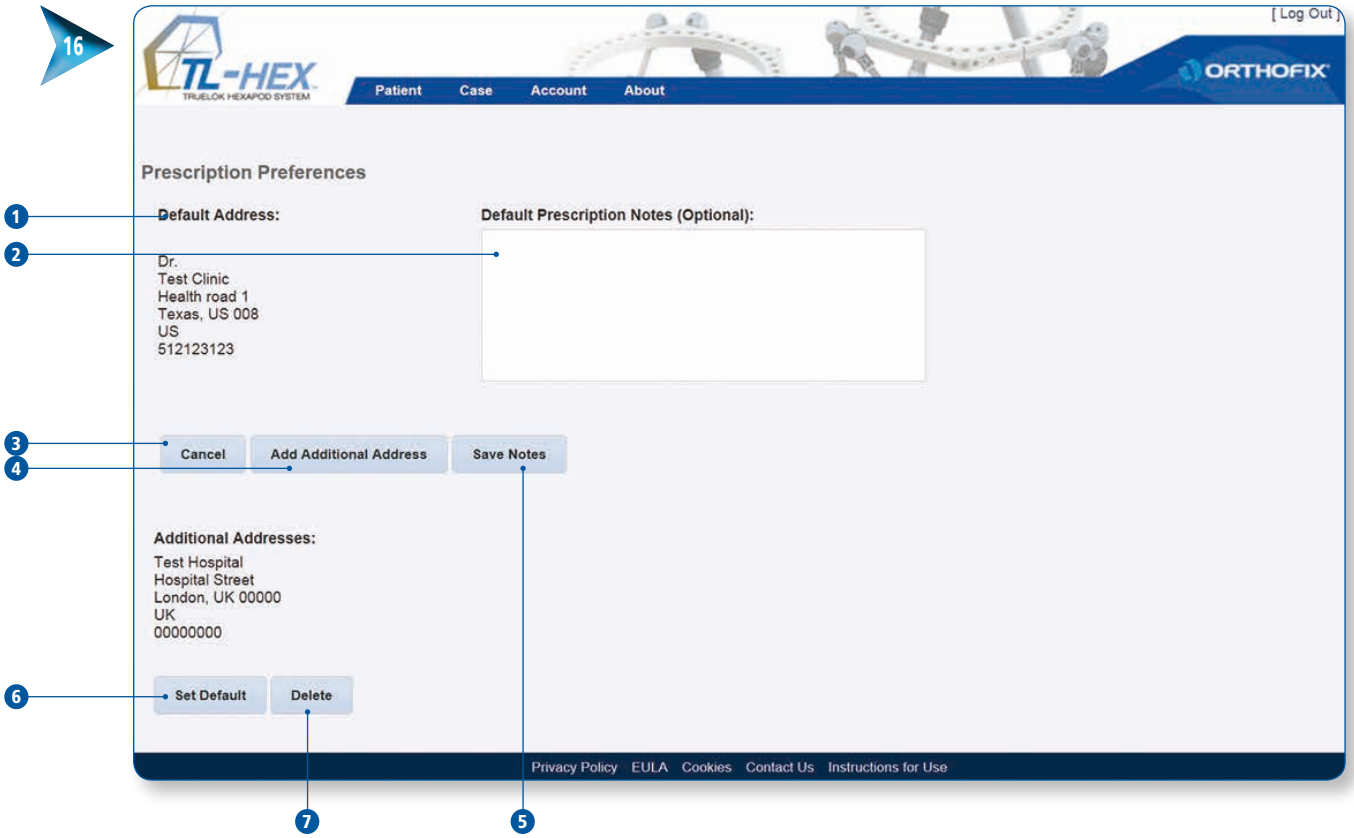
[Log Out]
TL-HEX
TRUELOK HEXAPOD SYSTEM
Patient
Case
Account
About
ORTHOFIX
Prescription Preferences
Default Address:
Dr.
Test Clinic
Health road 1
Texas, US 008
US
512123123
Default Prescription Notes (Optional):
Cancel
Add Additional Address
Save Notes
Additional Addresses:
Test Hospital
Hospital Street
London, UK 00000
UK
00000000
Set Default
Delete
Privacy Policy
EULA
Cookies
Contact Us
Instructions for Use
1
2
3
4
5
6
7

15. Account -> Change password	
	Description
1	Type the old password
2	Chose and type the new password. It must be 6 or more characters
3	Click [Cancel] to go back to the previous screen without applying any changes to the prescription preferences
4	Click [Cancel] to cancel the action and come back to the home page
5	Click [Change Password] to submit the password change

16. Account -> Prescription Preferences	
	Description
1	The address included as default in the header of the prescription pdf file
2	Optionally notes can be entered. they will be displayed on the header of the prescription pdf file
3	Confirm by typing the new password again. The software will validate that the two passwords match
4	Click [Add Additional Address] to add another address to the prescription preferences set. You can add up to 4 different addresses
5	Click [Save Note] to save the entered notes
6	Click [Set Default] of an entered address to change the default address with this one
7	Click [Delete] to eliminate an address

What is new in the 1.3 Release

1	Landing page: depending on the country the user will be automatically redirect to version 1.2 or 1.3

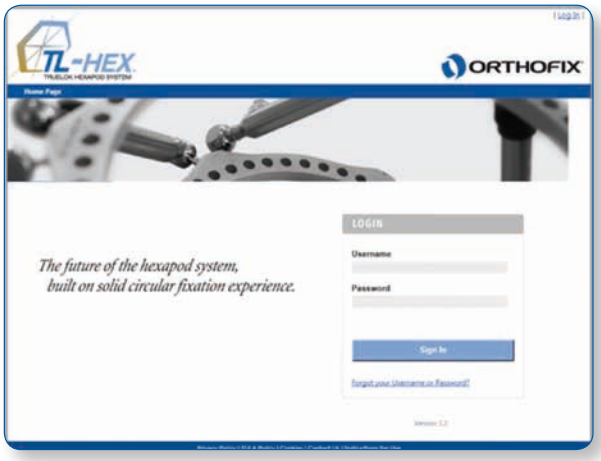

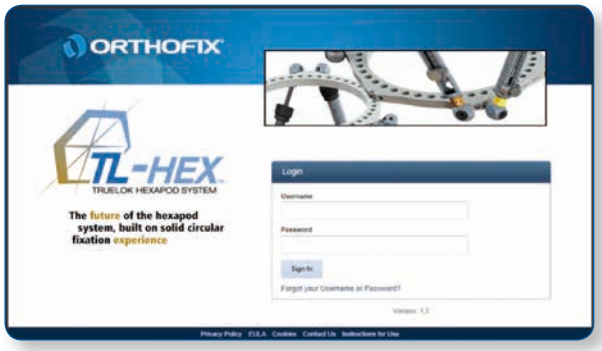

2	**Warning**: Cases done with the older sofwtare version will be **READ-ONLY**

3	Better look and Feel

New buttons to move to the next or previous screen

4	Preoperative option collapsed. The user can skip directly the preplanning if this option not used

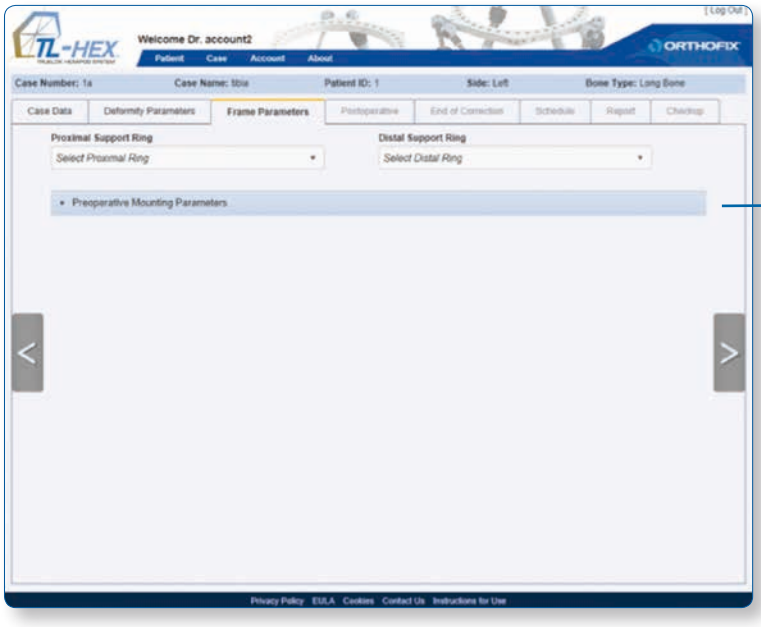

Preoperative option collapsed

5	"Apply first strut to all struts" button. This option copies applies the size, acute and gradual values of the first strut to all the others

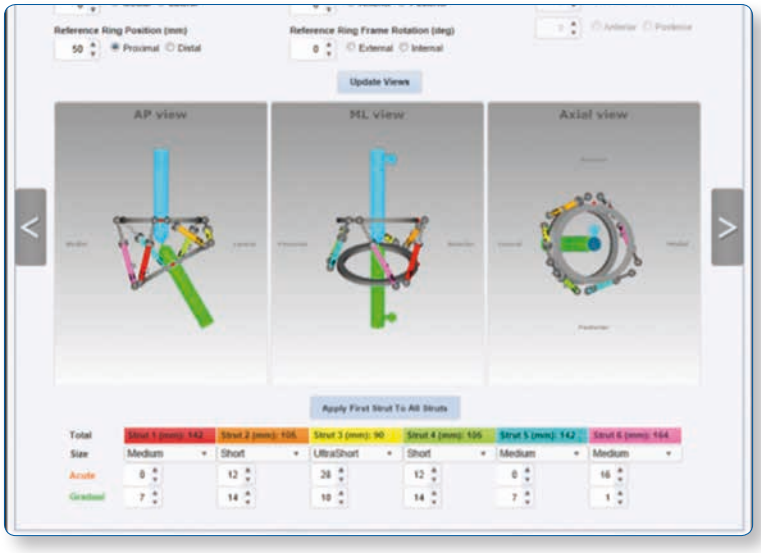

Apply first strut button to all struts

6	New foot option. The user can now plan a case also using a foot plate.

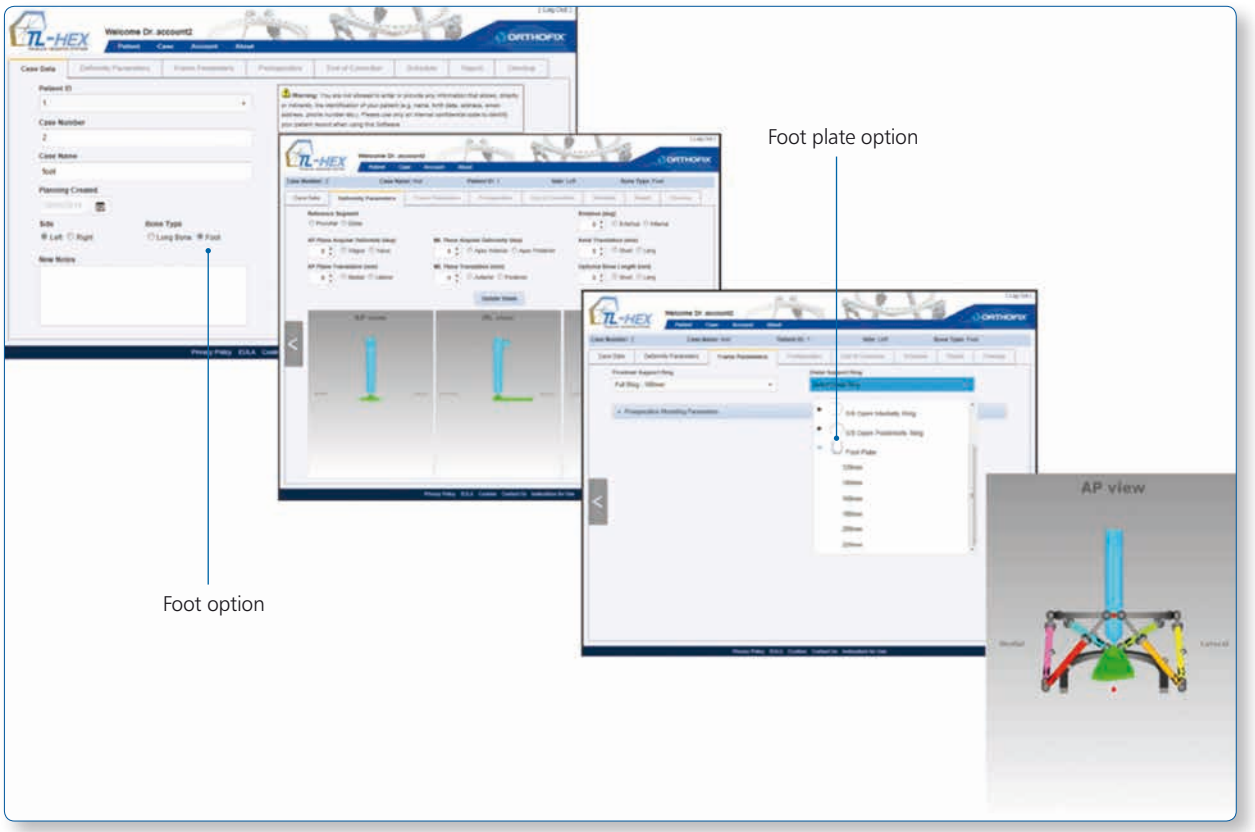

7	Better patients, cases visualtization and management. The possibility to archive and send a case to others users has been added

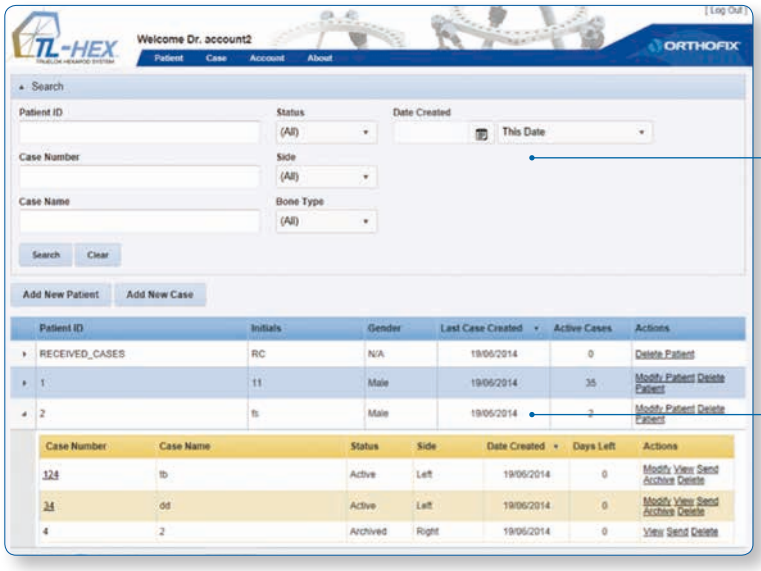

New and expanded searching options

Case options: Modify, View, Send, Archive, Delete

8	New prescription possibilities: the user can choose which address link to a patient selecting it from a set of up to 4 preferences.

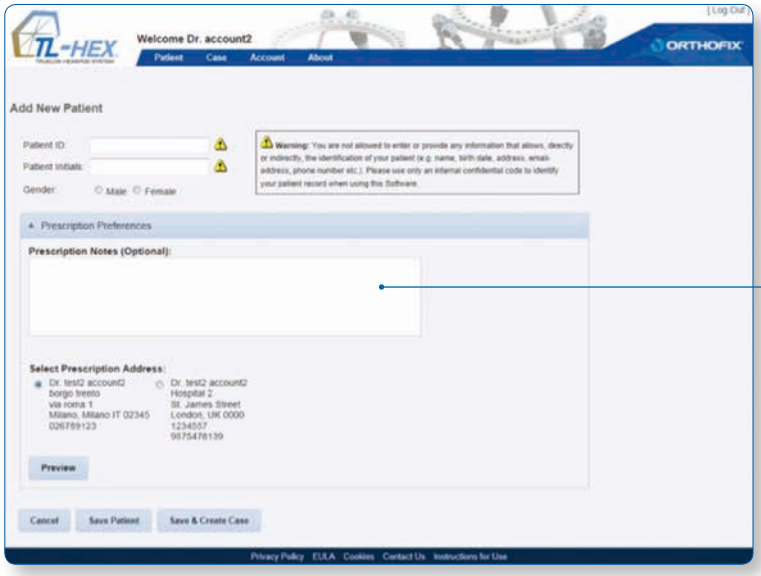

Option to add more references for the users

9	Simplified screen flow. The Prescription page has been incorporated in Report. A new option has been added "Print BOM" button (Bill of material). This button provides a list of all the TL-HEX codes used for the surgery including the struts necessary for later exchanges

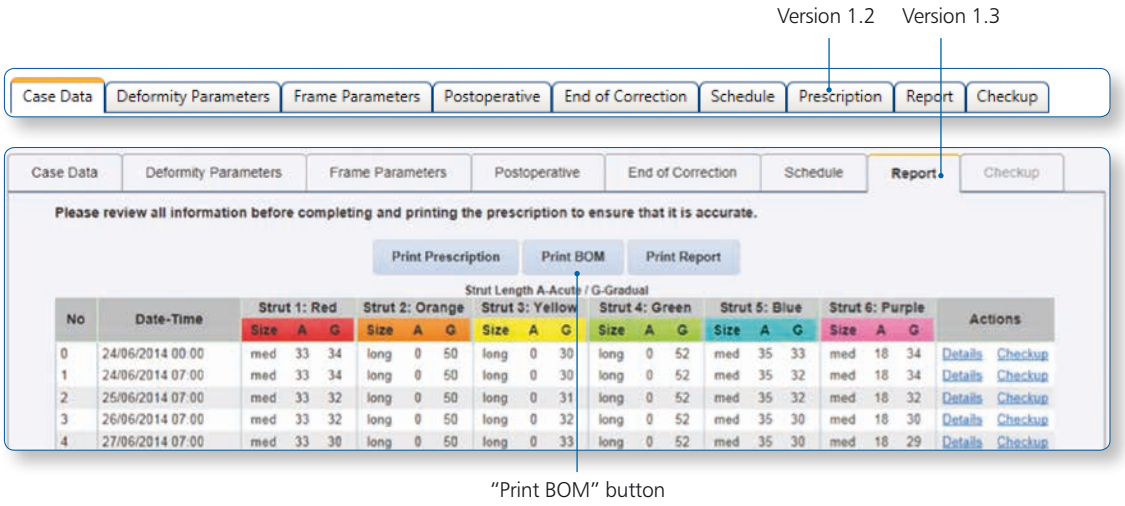

7	Improved printout for prescription in order to optimize the visualization also in black and white printers

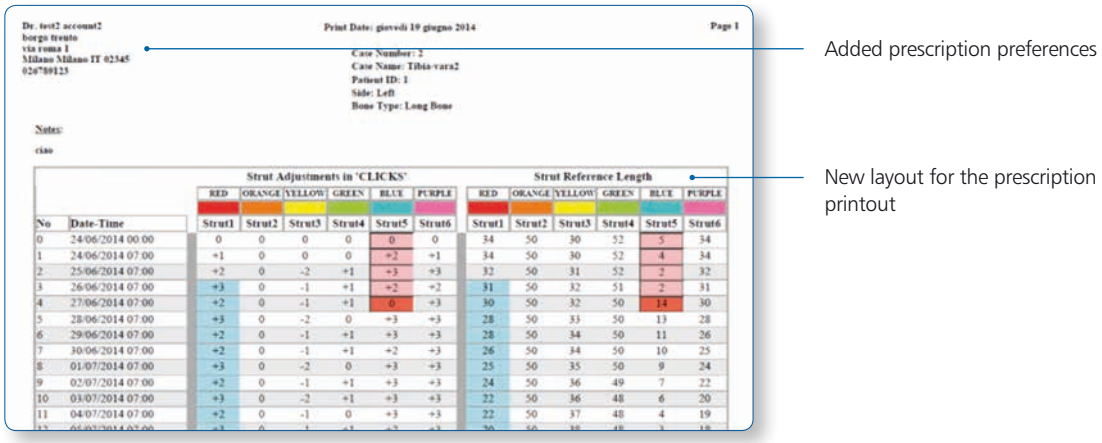

Manufactured by:
ORTHOFIX Srl
Via Delle Nazioni 9
37012 Bussolengo (Verona)
Italy

Telephone +39 045 6719000
Fax +39 045 6719380

CE

Your Distributor is:

www.orthofix.com
TL-1409-QR-E0 A 07/14

ORTHOFIX®